

# Calibrating Unit

## New Standard Solution Report

**ORIGINAL**

Sol. # 166

**Equipment** Alcotest 7110 MKIII-C  
Location: TOMS RIVER P.D.  
Calibration File No.: 01521  
Certification File No.: 01522  
Linearity File No.: 01523  
Solution File No.: 01578  
Sequential File No.: 01578

Serial No.: ARAJ-0075

2/5/15

Calib. Date: 11/05/2014  
Cert. Date: 11/05/2014  
Lin. Date: 11/05/2014  
Soln. Date: 02/05/2015  
File Date: 02/05/2015

Calib. No.: 00017  
Cert. No.: 00012  
Lin. No.: 00012  
Soln. No.: 00166

Calibrating Unit: WET  
Control Solution %: 0.100%  
Solution Control Lot: 14B127

Model No.: CU-34

Serial No.: DDWK S3-0386  
Expires: 02/14/2016  
Bottle No.: 0813

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:51S		
Control 1 EC	0.099%	17:52S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	17:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:53S		
Control 2 EC	0.098%	17:53S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	17:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:54S		
Control 3 EC	0.098%	17:55S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	17:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:55S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: MAIRE

First Name: GUY

MI: E

Signature: \_\_\_\_\_

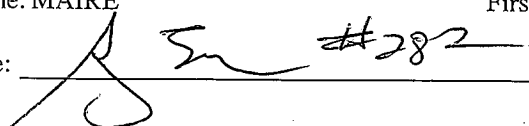

Badge No.: 1282

Date: 02/05/2015