

Calibrating Unit

 ORIGINAL

New Standard Solution Report

Sol. 174
6/3/2015

Equipment Alcotest 7110 MKIII-C Serial No.: ARAJ-0075
Location: TOMS RIVER P.D.
Calibration File No.: 01604 Calib. Date: 04/07/2015 Calib. No.: 00018
Certification File No.: 01605 Cert. Date: 04/07/2015 Cert. No.: 00013
Linearity File No.: 01606 Lin. Date: 04/07/2015 Lin. No.: 00013
Solution File No.: 01647 Soln. Date: 06/03/2015 Soln. No.: 00174
Sequential File No.: 01647 File Date: 06/03/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDAN-0041
Control Solution %: 0.100% Expires: 02/14/2016
Solution Control Lot: 14B127 Bottle No.: 0821

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:49D		
Control 1 EC	0.098%	13:50D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	13:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:50D		
Control 2 EC	0.097%	13:51D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	13:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:51D		
Control 3 EC	0.098%	13:52D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	13:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:53D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MAIRE

First Name: GUY

MI: E

Signature: _____

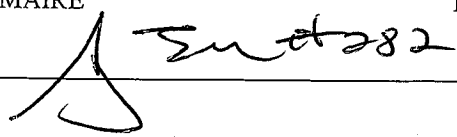

Badge No.: 1282

Date: 06/03/2015