

ORIGINAL

Calibrating Unit New Standard Solution Report

SOL. #180

7/31/15

Equipment Alcotest 7110 MKIII-C Serial No.: ARAJ-0075
Location: TOMS RIVER P.D.
Calibration File No.: 01604 Calib. Date: 04/07/2015 Calib. No.: 00018
Certification File No.: 01605 Cert. Date: 04/07/2015 Cert. No.: 00013
Linearity File No.: 01606 Lin. Date: 04/07/2015 Lin. No.: 00013
Solution File No.: 01686 Soln. Date: 07/31/2015 Soln. No.: 00180
Sequential File No.: 01686 File Date: 07/31/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDAN-0041
Control Solution %: 0.100% Expires: 02/11/2017
Solution Control Lot: 15B137 Bottle No.: 0915

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:59D		
Control 1 EC	0.098%	10:00D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	10:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:01D		
Control 2 EC	0.097%	10:01D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:02D		
Control 3 EC	0.098%	10:02D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	10:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:03D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MAIRE

First Name: GUY

MI: E

Signature: _____

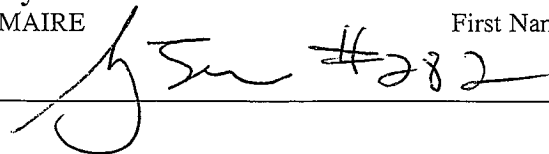

Badge No.: 1282

Date: 07/31/2015