

Calibrating Unit

New Standard Solution Report

ORIGINAL

SOL # 198

Equipment Alcotest 7110 MKIII-C
Location: TOMS RIVER P.D.
Calibration File No.: 01746
Certification File No.: 01747
Linearity File No.: 01748
Solution File No.: 01796
Sequential File No.: 01796

Serial No.: ARAJ-0075

Calib. Date: 10/02/2015
Cert. Date: 10/02/2015
Lin. Date: 10/02/2015
Soln. Date: 12/21/2015
File Date: 12/21/2015

Calib. No.: 00019
Cert. No.: 00014
Lin. No.: 00014
Soln. No.: 00198

12/21/15

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 15D138

Model No.: CU-34

Serial No.: DDAN-0041
Expires: 04/13/2017
Bottle No.: 0205

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:17S		
Control 1 EC	0.099%	15:17S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	15:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:18S		
Control 2 EC	0.099%	15:19S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	15:19S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:19S		
Control 3 EC	0.099%	15:20S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:20S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:21S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MAIRE

First Name: GUY

MI: E

Signature: _____

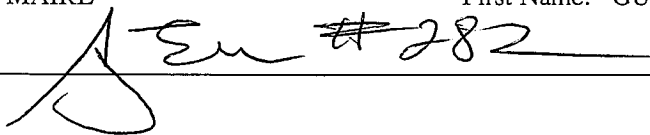

Badge No.: 1282

Date: 12/21/2015