

# Calibrating Unit New Standard Solution Report

Sol. # 226

8/13/16

**Equipment** Alcotest 7110 MKIII-C  
Location: TOMS RIVER P.D. Serial No.: ARWF-0394  
Calibration File No.: 01407 Calib. Date: 03/18/2016 Calib. No.: 00033  
Certification File No.: 01408 Cert. Date: 03/18/2016 Cert. No.: 00024  
Linearity File No.: 01409 Lin. Date: 03/18/2016 Lin. No.: 00024  
Solution File No.: 01474 Soln. Date: 08/13/2016 Soln. No.: 00226  
Sequential File No.: 01474 File Date: 08/13/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWK S3-0387  
Control Solution %: 0.100% Expires: 06/07/2018  
Solution Control Lot: 16140 Bottle No.: 1386

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:13D		
Control 1 EC	0.099%	14:13D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	14:13D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:14D		
Control 2 EC	0.098%	14:15D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	14:15D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:15D		
Control 3 EC	0.098%	14:16D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	14:16D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:17D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

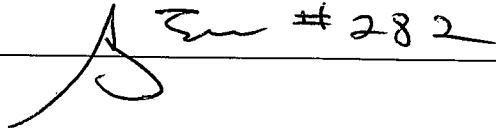
## Changed By:

Last Name: MAIRE

First Name: GUY

MI: E

Signature: \_\_\_\_\_

 # 282

Badge No.: 1282

Date: 08/13/2016