

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWF-0394
Location: TOMS RIVER P.D.
Calibration File No.: 01482 Calib. Date: 11/04/2016 Calib. No.: 00036
Certification File No.: 01483 Cert. Date: 11/04/2016 Cert. No.: 00026
Linearity File No.: 01484 Lin. Date: 11/04/2016 Lin. No.: 00026
Solution File No.: 01581 Soln. Date: 04/17/2017 Soln. No.: 00239
Sequential File No.: 01581 File Date: 04/17/2017

Calibrating Unit: WET Model No.: 41 Serial No.: DDAN-0040
Control Solution %: 0.100% Expires: 12/02/2018
Solution Control Lot: 16390 Bottle No.: 1305

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:47D		
Control 1 EC	0.097%	08:48D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	08:48D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:49D		
Control 2 EC	0.097%	08:49D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	08:49D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:50D		
Control 3 EC	0.097%	08:51D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	08:51D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:51D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: BARTOSHEK

First Name: DAVID

MI: G

Signature: _____

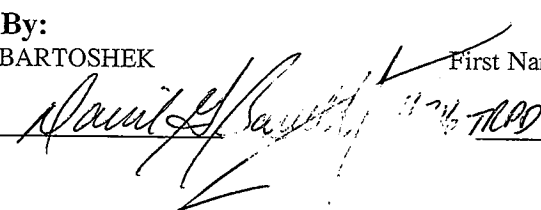

Badge No.: 316

Date: 04/17/2017