

Item 10  
**Alcotest 7110 Calibration Record**


<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARAJ-0075		
Location:	TOMS RIVER P.D.				
Calibration File No.:	02054	Calib. Date:	05/12/2017	Calib. No.:	00028
Certification File No.:	02043	Cert. Date:	04/18/2017	Cert. No.:	00018
Linearity File No.:	02044	Lin. Date:	04/18/2017	Lin. No.:	00018
Solution File No.:	02052	Soln. Date:	05/04/2017	Soln. No.:	00239
Sequential File No.:	02054	File Date:	05/12/2017		
Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDWK S3-0386
Control Solution %:	0.100%			Expires:	09/07/2018
Solution Control Lot:	16220			Bottle No.:	0100

**Coordinator**

Last Name:	ALCOTT	First Name:	KEVIN	MI:	W.
Signature:	<u><i>Tr. I K W. #6704</i></u>			Badge No.:	6704
				Date:	05/12/2017

\*Black Key Temperature Probe Serial.....# ΔΔXK P2 - 396 (KA)

\*Digital NIST Temperature Measuring System Serial.....# 150 649 672 (KA)

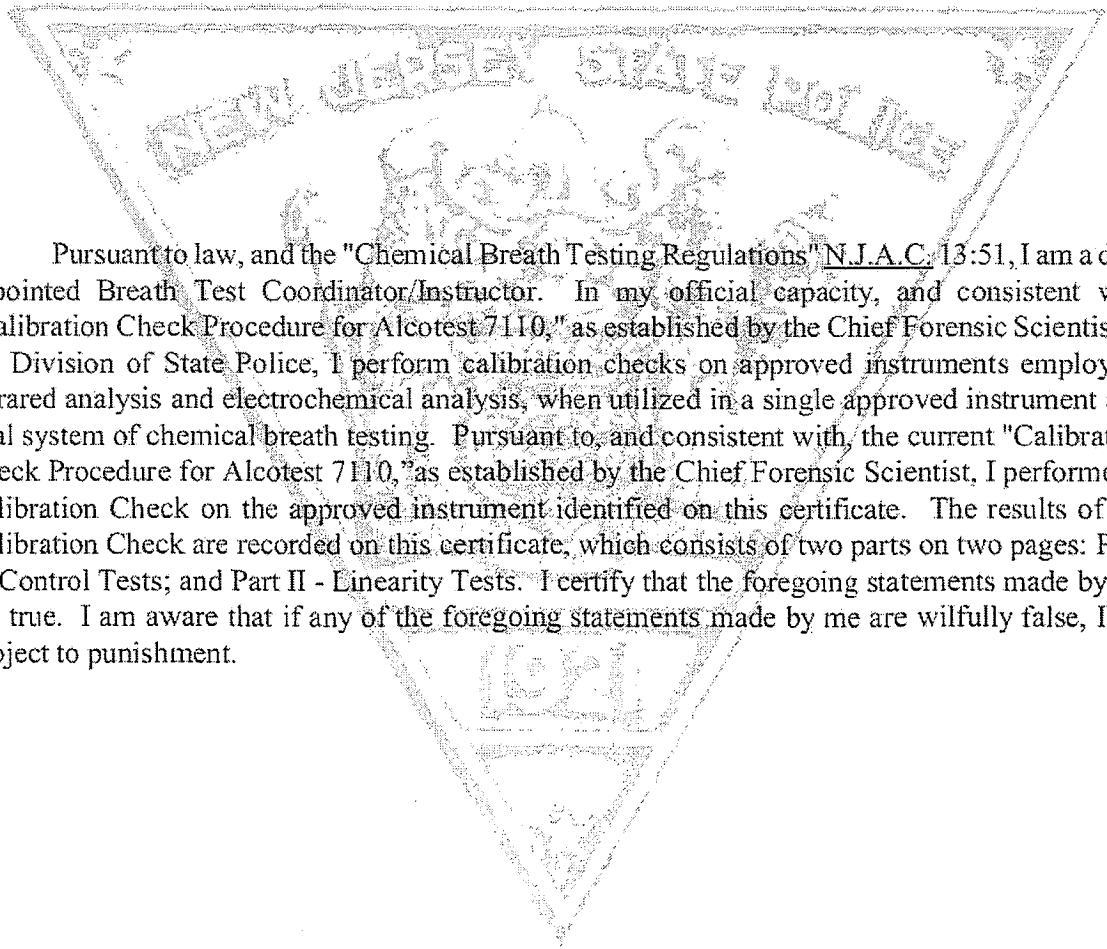

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.