

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARAJ-0075
Location:	TOMS RIVER P.D.		
Calibration File No.:	02535	Calib. Date:	12/27/2018
Certification File No.:	02536	Cert. No.:	00032
Linearity File No.:	02537	Cert. Date:	12/27/2018
Solution File No.:	02584	Lin. Date:	12/27/2018
Sequential File No.:	02584	Lin. No.:	00023
		Soln. Date:	03/01/2019
		Soln. No.:	00309
		File Date:	03/01/2019
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWK S3-0386
Solution Control Lot:	18150	Expires:	05/10/2020
		Bottle No.:	1303

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:26S		
Control 1 EC	0.100%	12:26S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	12:26S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:27S		
Control 2 EC	0.099%	12:28S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	12:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:29S		
Control 3 EC	0.097%	12:29S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:29S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:30S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: GAMBARDELLA

First Name: PASCAL

MI: M

Signature: \_\_\_\_\_

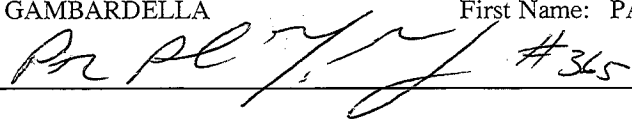

Badge No.: 365

Date: 03/01/2019