

Calibrating Unit ORIGINAL

New Standard Solution Report Sol. # 196

Equipment Alcotest 7110 MKIII-C
Location: TOMS RIVER P.D.
 Calibration File No.: 01221
 Certification File No.: 01222
 Linearity File No.: 01223
 Solution File No.: 01241
 Sequential File No.: 01241

Serial No.: ARWF-0394 2/14/15

Calib. Date: 11/05/2014 Calib. No.: 00028
 Cert. Date: 11/05/2014 Cert. No.: 00020
 Lin. Date: 11/05/2014 Lin. No.: 00020
 Soln. Date: 02/14/2015 Soln. No.: 00196
 File Date: 02/14/2015

FEB 16 2015

Calibrating Unit: WET
 Control Solution %: 0.100%
 Solution Control Lot: 14F130

Model No.: CU-34 Serial No.: DDWK S3-0387
 Expires: 06/20/2016
 Bottle No.: 0023

| Function | Result %BAC | Time HH:MM | Temperature Simulator (°C) | Comment(s) or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000% | 10:59S | | |
| Control 1 EC | 0.101% | 10:59S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.101% | 10:59S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 11:00S | | |
| Control 2 EC | 0.100% | 11:01S | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.100% | 11:01S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 11:02S | | |
| Control 3 EC | 0.100% | 11:02S | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.100% | 11:02S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 11:03S | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MAIRE

First Name: GUY

MI: E

Signature: _____

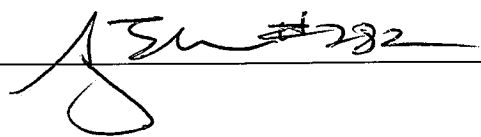

Badge No.: 1282

Date: 02/14/2015