

# Calibrating Unit New Standard Solution Report

 ORIGINAL

SD. # 217

**Equipment** Alcotest 7110 MKIII-C  
Location: TOMS RIVER P.D.  
Calibration File No.: 01324  
Certification File No.: 01325  
Linearity File No.: 01326  
Solution File No.: 01384  
Sequential File No.: 01384

Serial No.: ARWF-0394

2/24/16

Calib. Date: 10/02/2015  
Cert. Date: 10/02/2015  
Lin. Date: 10/02/2015  
Soln. Date: 02/24/2016  
File Date: 02/24/2016

Calib. No.: 00032  
Cert. No.: 00023  
Lin. No.: 00023  
Soln. No.: 00217

Calibrating Unit: WET  
Control Solution %: 0.100%  
Solution Control Lot: 15D138

Model No.: CU-34

Serial No.: DDWK S3-0387  
Expires: 04/13/2017  
Bottle No.: 0225

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:00S		
Control 1 EC	0.100%	16:01S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	16:01S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:01S		
Control 2 EC	0.100%	16:02S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	16:02S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:03S		
Control 3 EC	0.101%	16:03S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	16:03S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:04S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

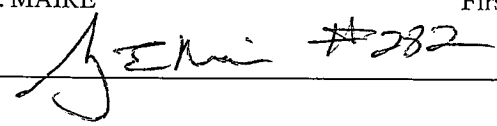
**Changed By:**

Last Name: MAIRE

First Name: GUY

MI: E

Signature: \_\_\_\_\_

 #282

Badge No.: 1282

Date: 02/24/2016