

ALCOTEST CERTIFICATIONS INDEX

03-18-2016

ARAJ-0075

- ITEM # 1 - NJSP OFFICER'S ALCOTEST CREDENTIALS
- ITEM # 2 - CERT OF ANALYSIS SIMULATOR SOLUTION 0.10
- ITEM # 3 - CERT OF ANALYSIS SIMULATOR SOLUTION 0.04
- ITEM # 4 - CERT OF ANALYSIS SIMULATOR SOLUTION 0.08
- ITEM # 5 - CERT OF ANALYSIS SIMULATOR SOLUTION 0.16
- ITEM # 6 - NIST CERT
- ITEM # 7 - ALCOTEST CU34 SERIAL #DDWES3-0206
- ITEM # 8 - ALCOTEST CU34 SERIAL #DDWFS3-0218
- ITEM # 9 - ALCOTEST CU34 SERIAL #DDWJS3-0334
- ITEM # 10 - ALCOTEST TEMPERATURE PROBE SERIAL # DDXKP2-396
- ITEM # 11 - TRPD ALCOTEST 7110 MK111-C SERIAL # ARAJ-0075
- ITEM # 12 - TRPD ALCOTEST CU34 SERIAL # DDWKS3-0386
- ITEM # 13 - TRPD ALCOTEST TEMP PROBE SERIAL # DDWJP2-025
- ITEM # 14 - ALCOTEST 7110 CALIBRATION RECORD
- ITEM # 15 - ALCOTEST 7110 CALIBRATION CONTROL TESTS
- ITEM # 16 - ALCOTEST 7110 CALIBRATION LINEARITY TESTS
- ITEM # 17 - NJSP NEW STANDARD SOLUTION REPORT
- ITEM # 18 - CERTIFICATE OF ANALYSIS SIMULATOR SOLUTION (15D138)
- ITEM # 19 - ALCOTEST CARDS/SOLUTION CHANGE OPERATOR (2PGS.)

ARAJ 0075

item 1 of 19

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Kevin W. Alcott
Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1966 IN THE OPERATION OF THE **Alcotest 7110 MKIII-C**
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 21st DAY OF May
TWO THOUSAND AND Fifteen

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ACTING ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 06/13)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

KEVIN W. ALCOTT
NEW JERSEY STATE POLICE

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1966 IN THE OPERATION OF THE **ALCOTEST 7110 MKIII-C**
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 18th DAY OF APRIL
TWO THOUSAND AND EIGHT

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 8-28-10	ALCPA	R. Fox
2. 1-12-12	BEVERLY LODGE	C. J.
3. 1-16-14	SAYREVILLE PD	R. Fox
4. 1/21/16	Lakehurst	Chris Stender
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 07/07)

item 2 of 19



ATAJ-0075

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

JOHN J. HOFFMAN
Acting Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

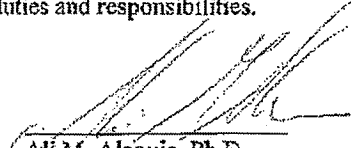
ANALYSIS DATE: 09/14/2015

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 15H143

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1198 to 0.1226 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 17, 2017.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 18th day of September, 2015.


MARY ELIZABETH MCLAUGHLIN

ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



item 3 of 19



Araj-0075

CHRIS CHRISTIE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

JOHN J. HOFFMAN
Acting Attorney General

KIM GUADAGNO
Lt. Governor

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

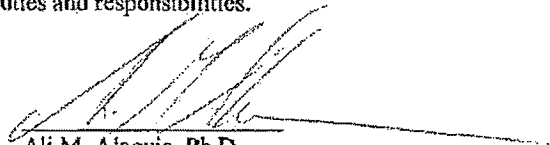
ANALYSIS DATE: 9/10/2015

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 15H141


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0478 to 0.0487 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 11, 2017.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Ali M. Alaoie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 11th day of September, 2015.


Notary
MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



item 4 of 19



Araj - 0075

CHRIS CHRISTIE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08626-0068
(609) 882-2000

JOHN J. HOFFMAN
Acting Attorney General

KIM GUADAGNO
Lt. Governor

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Dräger Safety, Inc.

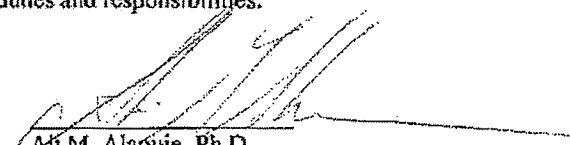
ANALYSIS DATE: 9/17/2015

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 15H142


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0959 to 0.0967 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 13, 2017.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Ali M. Aladine, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 18th day of September, 2015.


Notary
MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



item 5 of 19



Araj - 0075

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

JOHN J. HOFFMAN
Acting Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

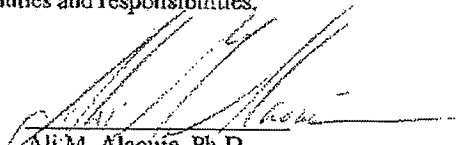
ANALYSIS DATE: 8/14/2014

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 14H131


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1925 to 0.1944 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 5, 2016.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 18th day of August, 2014.


Notary
MARY ELIZABETH MCLAUGHLIN
ID # 2052180
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



item 6 of 19



Calibration
Certificate No. 1750.01

Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001

Araj-0075



Cert. No.: 4000-7019762

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International, LLC, Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA 19087

Instrument Identification:

Model: 61220-601 S/N: 150649672 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath TC-256	B01375		
Temperature Probe	128	4/02/16	15-A0P2S-40-1
Thermistor Module	A17118	3/03/16	1000371058
Temperature Calibration Bath TC-179	A45240		
Thermistor Module	A17118	3/03/16	1000371058
Temperature Probe	3039	4/02/16	15-A0P2S-20-1
Temperature Calibration Bath TC-231	A79341		
Thermistor Module	A27129	11/04/15	1000365407
Temperature Probe	5202	11/19/16	6-CV9Y2-1-1
Temperature Calibration Bath TC-309	B3A444		
Thermistor Module	A27129	11/04/15	1000365407
Temperature Probe	5257	11/19/16	6-CV9Y0-1-1

Certificate Information:

Technician: 68 Procedure: CAL-06 Cal Date: 8/31/15 Due Date: 8/31/17
Test Conditions: 23.0°C 47.0 %RH 1017 mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C		N.A.		0.001	0.000	Y	-0.049	0.051	0.013	3.8:1
°C		N.A.		25.000	25.003	Y	24.950	25.050	0.014	3.6:1
°C		N.A.		50.004	50.000	Y	49.954	50.054	0.014	3.6:1
°C		N.A.		100.002	99.999	Y	99.952	100.052	0.014	3.6:1

This Instrument was calibrated using Instruments Traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min = As Left Nominal(Rounded) - Tolerance; Max = As Left Nominal(Rounded) + Tolerance; Date=MM/DD/YY

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Aaron Judice
Aaron Judice, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:


For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 4455 Rex Road Friendswood, TX 77546 USA
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (AZLA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-2008-AQ-HOU-RVA.
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).

item 7 of 19

-Araj-0075



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- ☒ Model: ALCOTEST® CU34
☐ Model: MARK IIA
☐ Other: _____

Serial Number:

DDWES3-0206

Certification Date

10-30-15

Technician


72

Re-Certification Due Date

10-30-16

item 8 of 19

Araj-0075



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- ☒ Model: ALCOTEST® CU34
☐ Model: MARK IIA
☐ Other: _____

Serial Number:

DDWFS3-0218

Certification Date

10-30-15

Technician


72

Re-Certification Due Date

10-30-16

item 9 of 19

Araj-0075



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

☒ Model: ALCOTEST® CU34

☐ Model: MARK IIA

☐ Other: _____

Serial Number:

DDWJS3-0334

Certification Date

10-30-15

Technician

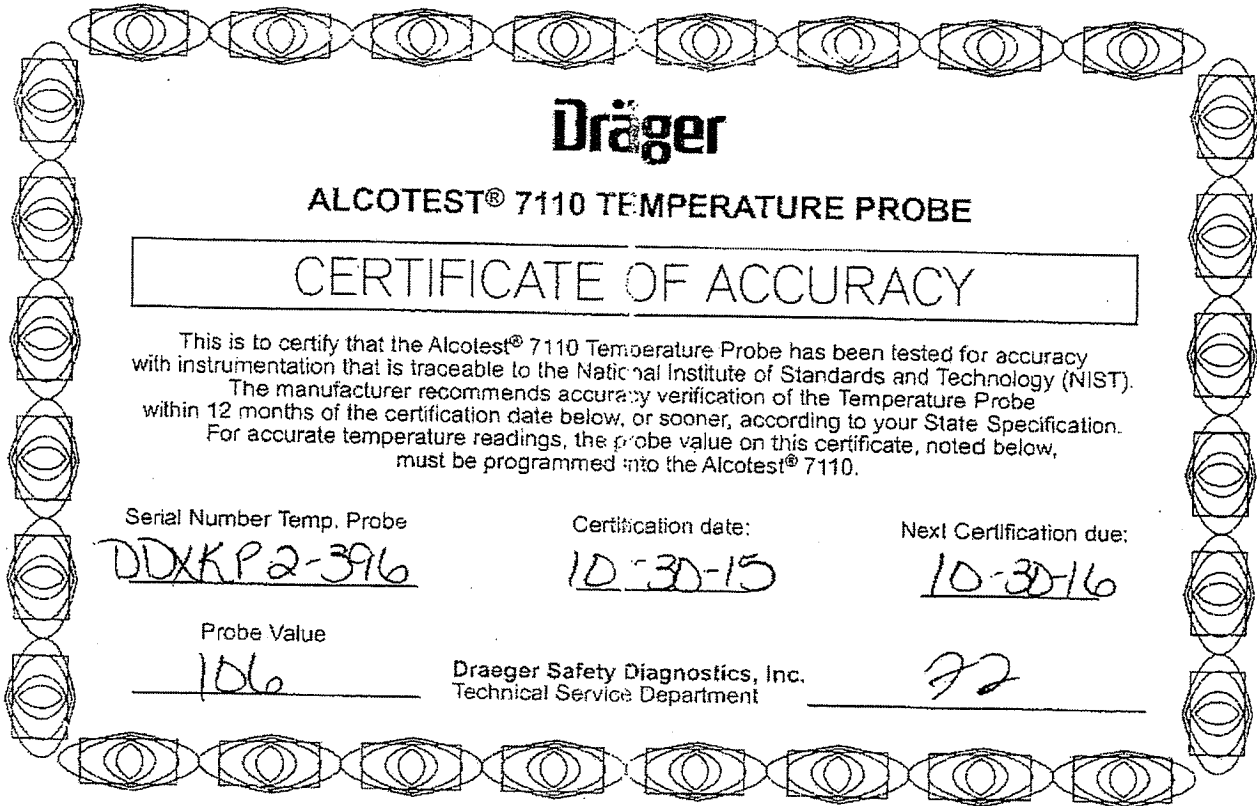
72

Re-Certification Due Date

10-30-16

item 10 of 19

— ARAJ-0075



Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe	Certification date:	Next Certification due:
<u>DDXKP2-396</u>	<u>10-30-15</u>	<u>10-30-16</u>
Probe Value	Dräger Safety Diagnostics, Inc.	
<u>106</u>	Technical Service Department	
		<u>72</u>

item 11 of 19

ARAJ-0075

Dräger

Alcotest® 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

3-4-16

SERIAL NUMBER:


ARAJ-0075

Draeger Safety Diagnostics, Inc.

BC

item 12 of 19

- Aray - 0075



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- ☒ Model: ALCOTEST® CU34
☐ Model: MARK IIA
☐ Other: _____

Serial Number:

DDWKS3 - 0386

Certification Date

1-29-16

Technician


JD

Re-Certification Due Date

1-29-17

item 13 of 19

ARAJ-0075



ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe, within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe	Certification date:	Next Certification due:
<u>DDWJP2-025</u>	<u>1-27-16</u>	<u>1-27-17</u>
Probe Value	Draeger Safety Diagnostics, Inc. Technical Service Department	<u>72</u>
<u>102</u>		

?

item 14 of 19

Alcotest 7110 Calibration Record

ARAJ-0075

Equipment

Alcotest 7110 MKIII-C
Location: TOMS RIVER P.D.
Calibration File No.: 01818
Certification File No.: 01747
Linearity File No.: 01748
Solution File No.: 01817
Sequential File No.: 01818

Calib. Date: 03/18/2016
Cert. Date: 10/02/2015
Lin. Date: 10/02/2015
Soln. Date: 03/04/2016
File Date: 03/18/2016

Serial No.: ARAJ-0075

Calib. No.: 00021
Cert. No.: 00014
Lin. No.: 00014
Soln. No.: 00204

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 15H143

Model No.: CU-34

Serial No.: DDWK S3-0386
Expires: 08/17/2017
Bottle No.: 1056

Coordinator

Last Name: ALCOTT

First Name: KEVIN

MI: W.

Signature: Tpr. I K W G #6704

Badge No.: 6704

Date: 03/18/2016

*Black Key Temperature Probe Serial.....#

DDXKPZ - 396

(KA)

*Digital NIST Temperature Measuring System Serial.....#

150 649 672

(KA)

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

item 15 of 19

Alcotest 7110 Calibration Certificate

Part I - Control Tests

ARAJ-0075

Equipment Alcotest 7110 MKIII-C
Location: TOMS RIVER P.D.
Calibration File No.: 01818
Certification File No.: 01819
Linearity File No.: 01748
Solution File No.: 01817
Sequential File No.: 01819

Calib. Date: 03/18/2016
Cert. Date: 03/18/2016
Lin. Date: 10/02/2015
Soln. Date: 03/04/2016
File Date: 03/18/2016

Serial No.: ARAJ-0075

Calib. No.: 00021
Cert. No.: 00015
Lin. No.: 00014
Soln. No.: 00204

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 15H143

Model No.: CU-34

Serial No.: DDWK S3-0386
Expires: 08/17/2017
Bottle No.: 1056

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:27S	09:27 Δ KA	
Control 1 EC	0.099%	08:28S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:28S		
Control 2 EC	0.099%	08:29S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:29S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:29S		
Control 3 EC	0.100%	08:30S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:30S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:30S	09:30 Δ KA	

All tests within acceptable tolerance.

Coordinator

Last Name: ALCOTT

First Name: KEVIN

MI: W.

Signature:

Tpt. I K W g #6704

Badge No.: 6704

Date: 03/18/2016

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

item 16 of 19

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

ARAJ-0075

Equipment Alcotest 7110 MKIII-C Serial No.: ARAJ-0075
Location: TOMS RIVER P.D.
Calibration File No.: 01818 **Calib. Date:** 03/18/2016 **Calib. No.:** 00021
Certification File No.: 01819 **Cert. Date:** 03/18/2016 **Cert. No.:** 00015
Linearity File No.: 01820 **Lin. Date:** 03/18/2016 **Lin. No.:** 00015
Solution File No.: 01817 **Soln. Date:** 03/04/2016 **Soln. No.:** 00204
Sequential File No.: 01820 **File Date:** 03/18/2016

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDWE S3-0206
Control Solution %: 0.040% **Expires:** 08/11/2017
Solution Control Lot: 15H141 **Bottle No.:** 0800

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDWF S3-0218
Control Solution %: 0.080% **Expires:** 08/13/2017
Solution Control Lot: 15H142 **Bottle No.:** 1026

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDWJ S3-0334
Control Solution %: 0.160% **Expires:** 08/05/2016
Solution Control Lot: 14H131 **Bottle No.:** 0375

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:47S	09:47 Δ KA	
Control 1 EC	0.039%	08:47S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.040%	08:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:49S		
Control 2 EC	0.041%	08:49S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.040%	08:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:51S		
Control 3 EC	0.079%	08:51S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.079%	08:51S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:53S		
Control 4 EC	0.079%	08:53S	34.0°C	*** TEST PASSED ***
Control 4 IR	0.080%	08:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:54S		
Control 5 EC	0.156%	08:55S	34.0°C	*** TEST PASSED ***
Control 5 IR	0.155%	08:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:57S		
Control 6 EC	0.157%	08:57S	33.9°C	*** TEST PASSED ***
Control 6 IR	0.156%	08:57S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:59S	09:59 Δ KA	

All tests within acceptable tolerance.

Coordinator

Last Name: ALCOTT

First Name: KEVIN

MI: W.

Signature:

Tpr. I RK W. #6704

Badge No.: 6704

Date: 03/18/2016

item 17 of 19

Calibrating Unit
New Standard Solution Report

ARAJ-0075

Sol. # 205

3-18-16

Equipment Alcotest 7110 MKIII-C
Location: TOMS RIVER P.D.
Calibration File No.: 01818
Certification File No.: 01819
Linearity File No.: 01820
Solution File No.: 01821
Sequential File No.: 01821

Calib. Date: 03/18/2016
Cert. Date: 03/18/2016
Lin. Date: 03/18/2016
Soln. Date: 03/18/2016
File Date: 03/18/2016

Serial No.: ARAJ-0075

Calib. No.: 00021
Cert. No.: 00015
Lin. No.: 00015
Soln. No.: 00205

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 15D138

Model No.: CU-34

Serial No.: DDWK S3-0386
Expires: 04/13/2017
Bottle No.: 0221

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:11S	11:11 Δ KA	
Control 1 EC	0.101%	10:11S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:11S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:12S		
Control 2 EC	0.101%	10:13S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:13S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:13S		
Control 3 EC	0.101%	10:14S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:14S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:14S	11:14 Δ KA	

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: ΔΔWJPZ-025 (KA)

Changed By:

Last Name: ALCOTT

First Name: KEVIN

MI: W.

Signature: TP. I K W. 9 #6704

Badge No.: 6704

Date: 03/18/2016

item 18 of 19



Araj-0075

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

JOHN J. HOFFMAN
Acting Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 5/6/2015

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 15D138

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1203 to 0.1220 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is April 13, 2017.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 7th day of may, 2015.

Notary
MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



Item 19 of 19

ARAJ-0075

DEPARTMENT OF
Traffic and Public Safety
This is to certify that
Guy E. Maine
Dover Township

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE ALCOTEST 7110 MKIII-C
A METHOD TO DETERMINE INTOXICATION
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 23rd DAY OF November
TWO THOUSAND AND FIVE

[Signature] SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature] ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 11/29/07	OCPA	[Signature]
2. 7/4/09	OCPA	[Signature]
3. 2-22-11	OCPA	Wm Linn
4. 1-28-13	OCPA	Wm Linn
5. 3/4/15	OCPA	Adam Standa
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 06/03)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that
Timothy M. Sysol
Dover Township

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE ALCOTEST 7110 MKIII-C
A METHOD TO DETERMINE INTOXICATION
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 7th DAY OF December
TWO THOUSAND AND FIVE

[Signature] SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature] ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 12-10-07	OCPA	Wm Linn
2. 7-30-09	OCPA	Wm Linn
3. 1-31-11	OCPA	Wm Linn
4. 1-22-13	OCPA	Wm Linn
5. 2-4-15	OCPA	Wm Linn
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 06/03)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that
Kenneth J. Thomas Jr.
Toms River Township

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 7110 MKIII-C
A METHOD TO DETERMINE INTOXICATION
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 3rd DAY OF September
TWO THOUSAND AND NINE

[Signature] SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature] ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 1-18-11	OCPA	Wm Linn
2. 1-22-13	OCPA	Wm Linn
3. 2-4-15	OCPA	Wm Linn
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 07/07)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that
Christopher W. Anderson
Toms River Police Department

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE ALCOTEST 7110 MK III-C
A METHOD TO DETERMINE INTOXICATION
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 13th DAY OF November
TWO THOUSAND AND Seven

[Signature] SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature] ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES 11-28-2005

DATE	Refresher Course PLACE	INSTRUCTOR
1. 11/28/07	OCPA	[Signature]
2. 12/4/09	OCPA	[Signature]
3. 1-3-11	OCPA	Wm Linn
4. 9/4/13	CMPA	Adam Standa
5. 1-20-15	OCPA	Wm Linn
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 07/07)

item 19 of 19

ARAJ-0075

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

David Bartoshek
Toms River Township Police Department

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE ALCOTEST 7110 MK III-C
A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 28th DAY OF February
TWO THOUSAND AND FOURTEEN

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Robert Westfall
Toms River Township Police Department

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE ALCOTEST 7110 MK III-C
A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 4th DAY OF June
TWO THOUSAND AND TEN

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Adam M. Koeppe
Toms River Township

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE ALCOTEST 7110 MK III-C
A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 31st DAY OF March
TWO THOUSAND AND ELEVEN

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES 1/3/2006

DATE	Refresher Course PLACE	INSTRUCTOR
1. <u>1/6/2014</u>	<u>Lakehurst</u>	<u>Cross</u>
2. <u>2-16-16</u>	<u>LAKEHURST</u>	<u>Gum Coon</u>
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 293B (Rev. 08/13)

ORIGINAL COURSE DATES 1/4/2006

DATE	Refresher Course PLACE	INSTRUCTOR
1. <u>2/8/2010</u>	<u>Ocean Co. P.A.</u>	<u>Stanks</u>
2. <u>1/5/11</u>	<u>OC PA</u>	<u>Adam Stanks</u>
3. <u>1-29-13</u>	<u>OC PA</u>	<u>Wm Coon</u>
4. <u>3-2-15</u>	<u>O CPA</u>	<u>Wm Coon</u>
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 293B (Rev. 03/10)

ORIGINAL COURSE DATES _____

DATE	Refresher Course PLACE	INSTRUCTOR
1. <u>1/17/13</u>	<u>OLPA</u>	<u>Adam Stanks</u>
2. <u>1-22-15</u>	<u>OLPA</u>	<u>Wm Coon</u>
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 293B (Rev. 03/10)