

item 14 of 19

Alcotest 7110 Calibration Record *ARAJ-0075*

Equipment

Alcotest 7110 MKIII-C
 Location: TOMS RIVER P.D.
 Calibration File No.: 01818
 Certification File No.: 01747
 Linearity File No.: 01748
 Solution File No.: 01817
 Sequential File No.: 01818

Serial No.: ARAJ-0075

Calib. Date: 03/18/2016 Calib. No.: 00021
 Cert. Date: 10/02/2015 Cert. No.: 00014
 Lin. Date: 10/02/2015 Lin. No.: 00014
 Soln. Date: 03/04/2016 Soln. No.: 00204
 File Date: 03/18/2016

Calibrating Unit: WET
 Control Solution %: 0.100%
 Solution Control Lot: 15H143

Model No.: CU-34

Serial No.: DDWK S3-0386
 Expires: 08/17/2017
 Bottle No.: 1056

Coordinator

Last Name: ALCOTT

First Name: KEVIN

MI: W.


Signature: *Tpt. I K W of #6704*

Badge No.: 6704

Date: 03/18/2016

*Black Key Temperature Probe Serial.....# *DDXKPZ - 396* (KA)

*Digital NIST Temperature Measuring System Serial.....# *150 649 672* (KA)

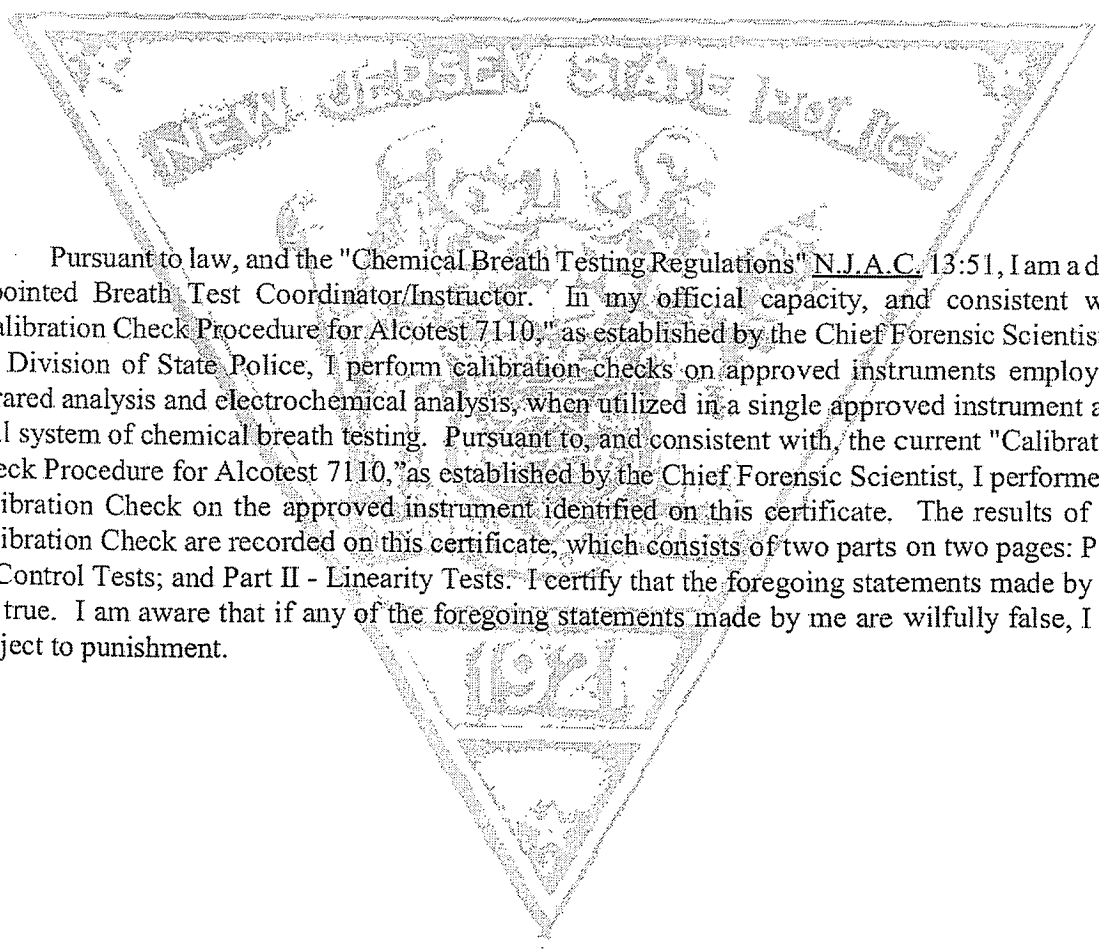

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.