

Calibrating Unit

New Standard Solution Report

SOI-217
8/13/16

Equipment Alcotest 7110 MKIII-C
Location: TOMS RIVER P.D.
Calibration File No.: 01818
Certification File No.: 01819
Linearity File No.: 01820
Solution File No.: 01921
Sequential File No.: 01921

Serial No.: ARAJ-0075

Calib. Date: 03/18/2016
Cert. Date: 03/18/2016
Lin. Date: 03/18/2016
Soln. Date: 08/13/2016
File Date: 08/13/2016

Calib. No.: 00021
Cert. No.: 00015
Lin. No.: 00015
Soln. No.: 00217

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 16140

Model No.: CU-34

Serial No.: DDWK S3-0386
Expires: 06/07/2018
Bottle No.: 1204

| Function | Result %BAC | Time HH:MM | Temperature Simulator (°C) | Comment(s) or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000% | 14:31D | | |
| Control 1 EC | 0.098% | 14:32D | 33.9°C | *** TEST PASSED *** |
| Control 1 IR | 0.099% | 14:32D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:33D | | |
| Control 2 EC | 0.097% | 14:33D | 33.9°C | *** TEST PASSED *** |
| Control 2 IR | 0.098% | 14:33D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:34D | | |
| Control 3 EC | 0.098% | 14:34D | 33.9°C | *** TEST PASSED *** |
| Control 3 IR | 0.098% | 14:34D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:35D | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

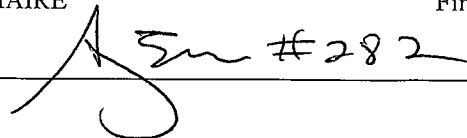
Changed By:

Last Name: MAIRE

First Name: GUY

MI: E

Signature: _____

 #282

Badge No.: 1282

Date: 08/13/2016