

ALCOTEST CERTIFICATIONS INDEX

9-15-2017

(11-22-2017 = ADDENDUM)

ARAJ-0075

- ITEM # 1 - NJSP OFFICER'S ALCOTEST CREDENTIALS
- ITEM # 2 - CERT OF ANALYSIS SIMULATOR SOLUTION 0.10
- ITEM # 3 - CERT OF ANALYSIS SIMULATOR SOLUTION 0.04
- ITEM # 4 - CERT OF ANALYSIS SIMULATOR SOLUTION 0.08
- ITEM # 5 - CERT OF ANALYSIS SIMULATOR SOLUTION 0.16
- ITEM # 6 - NIST CERT
- ITEM # 7 - ALCOTEST CU34 SERIAL #DDMKS3-0003
 - ALCOTEST CU34 SERIAL #DDRKS3-0024
- ITEM # 8 - ALCOTEST CU34 SERIAL #DDWES3-0203
(ADDENDUM = DDAN-0041)
 - ALCOTEST TEMPERATURE PROBE SERIAL # DDHHP2-065
(ADDENDUM = DDXKP2-436)
- ITEM # 9 - TRPD ALCOTEST 7110 MK111-C SERIAL # ARAJ-0075
- ITEM # 10 - TRPD ALCOTEST CU34 SERIAL # DDWK53-0386
 - TRPD ALCOTEST TEMP PROBE SERIAL # DDWJPL-025
- ITEM # 11 - ALCOTEST 7110 CALIBRATION RECORD
- ITEM # 12 - ALCOTEST 7110 CALIBRATION CONTROL TESTS
- ITEM # 13 - ALCOTEST 7110 CALIBRATION LINEARITY TESTS
- ITEM # 14 - NJSP NEW STANDARD SOLUTION REPORT
- ITEM # 15 - CERTIFICATE OF ANALYSIS SIMULATOR SOLUTION (17110)
- ITEM # 16 - ALCOTEST CARDS/SOLUTION CHANGE OPERATOR (3PGS.)

ALCOTEST CERTIFICATIONS INDEX

9-15-2017

ARAJ-0075

- ITEM # 1 - NJSP OFFICER'S ALCOTEST CREDENTIALS
- ITEM # 2 - CERT OF ANALYSIS SIMULATOR SOLUTION 0.10
- ITEM # 3 - CERT OF ANALYSIS SIMULATOR SOLUTION 0.04
- ITEM # 4 - CERT OF ANALYSIS SIMULATOR SOLUTION 0.08
- ITEM # 5 - CERT OF ANALYSIS SIMULATOR SOLUTION 0.16
- ITEM # 6 - NIST CERT
- ITEM # 7 - ALCOTEST CU34 SERIAL #DDMKS3-0003
 - ALCOTEST CU34 SERIAL #DDRKS3-0024
- ITEM # 8 - ALCOTEST CU34 SERIAL #DDWES3-0203
 - ALCOTEST TEMPERATURE PROBE SERIAL # DDHHP2-065
- ITEM # 9 - TRPD ALCOTEST 7110 MK111-C SERIAL # ARAJ-0075
- ITEM # 10 - TRPD ALCOTEST CU34 SERIAL # DDWK53-0386
 - TRPD ALCOTEST TEMP PROBE SERIAL # DDWJPL-025
- ITEM # 11 - ALCOTEST 7110 CALIBRATION RECORD
- ITEM # 12 - ALCOTEST 7110 CALIBRATION CONTROL TESTS
- ITEM # 13 - ALCOTEST 7110 CALIBRATION LINEARITY TESTS
- ITEM # 14 - NJSP NEW STANDARD SOLUTION REPORT
- ITEM # 15 - CERTIFICATE OF ANALYSIS SIMULATOR SOLUTION (17110)
- ITEM # 16 - ALCOTEST CARDS/SOLUTION CHANGE OPERATOR (3PGS.)



NEW JERSEY STATE POLICE
Alcohol Drug Testing Unit

Tpr. I KEVIN W. ALCOTT #6704

Hamilton Technology Complex
Suite #400
1200 Negron Drive
Hamilton, NJ 08691


Tel#: (609) 218-3345
Email: Lpp6704@gw.njsp.org


ITEM 1

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Kevin W. Alcott
Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1966 IN THE OPERATION OF THE **Alcotest 7110 MKIII-C**
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, 21st DAY OF May
THO THOUSAND AND Fifteen


SUPERINTENDENT
NEW JERSEY STATE POLICE


ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES


DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		


S.P. 202B (Rev. 06/13)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

KEVIN W. ALCOTT
NEW JERSEY STATE POLICE

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1966 IN THE OPERATION OF THE **ALCOTEST 7110 MKIII-C**
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, 18th DAY OF APRIL
THO THOUSAND AND EIGHT


SUPERINTENDENT
NEW JERSEY STATE POLICE


ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. <u>8-25-10</u>	<u>BCPA</u>	<u>R. Tan</u>
2. <u>1-12-12</u>	<u>Berwyn WPA</u>	<u>C. Tan</u>
3. <u>1-16-14</u>	<u>SAYREVILLE PD</u>	<u>R. Tan</u>
4. <u>1/21/16</u>	<u>Lakewood</u>	<u>Adam Gaudin</u>
5.		
6.		
7.		
8.		
9.		

S.P. 202B (Rev. 07/07)

ITEM 2



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

CHRISTOPHER S. PORRINO
Attorney General

KIM GUADAGNO
Lt. Governor

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Dräger Safety, Inc.


ANALYSIS DATE: 09/19/2016

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 16220

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1202 to 0.1207 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 07, 2018.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Ali M. Alnoute, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 27th day of September, 2016.


Notary

MARY ELIZABETH MCLAUGHLIN

ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS 0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Dräger Safety, Inc.


ANALYSIS DATE: 09/27/2016

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 16230

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0484 to 0.0492 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 19, 2018.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28th day of September, 2016.

Notary

MARY ELIZABETH MCLAUGHLIN

ID # 2062190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



Item 4



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

CHRISTOPHER S. PORRINO
Attorney General

KIM GUADAGNO
Lt. Governor

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.


ANALYSIS DATE: 10/04/2016

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 16250


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0965 to 0.0975 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 27, 2018.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 5th day of October, 2016.


Notary

MARY ELIZABETH MCLAUGHLIN

ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



ITEM 5



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

CHRISTOPHER S. PORRINO
Attorney General

KIM GUADAGNO
Lt. Governor

COLONEL JOSEPH R. PUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/13/2016

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 16260

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1928 to 0.1964 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is October 3, 2018.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 17 day of October, 2016.

Notary
JOHN R. LEAVER
ID # 2207138
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 14, 2017



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer.
Printed on Recycled Paper and Recyclable



ITEM 6



Calibration
Certificate No. 1750.01

Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-8609168

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International, LLC, Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA 19087

Instrument Identification:

Model: 61220-601 S/N: 170428368 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath TC-231	A79341		
Thermistor Module	A27129	12/01/17	1000401760
Temperature Probe	5267	12/06/17	B6B30059
Temperature Calibration Bath TC-191	A42238		
Thermistor Module	A27129	12/01/17	1000401760
Temperature Probe	5202	12/19/17	B6B30058-1
Temperature Calibration Bath TC-218	A73332		
Thermistor Probe	5356	1/10/18	B7104024
Readout, Digital Thermometer	B5C344	3/12/18	B7314035
Temperature Calibration Bath TC-275	B16388		
Thermistor Probe	5357	1/06/18	B7104023
Readout, Digital Thermometer	B5C344	3/12/18	B7314035

Certificate Information:

Technician: 104 Procedure: CAL-06 Cal Date: 6/08/17 Due Date: 6/08/19
Test Conditions: 23.5°C 50.0 %RH 1014 mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C		N.A.		0.002	0.001	Y	-0.048	0.052	0.010	>4.1
°C		N.A.		25.003	25.000	Y	24.953	25.053	0.010	>4.1
°C		N.A.		50.002	50.001	Y	49.952	50.052	0.010	>4.1
°C		N.A.		100.001	99.998	Y	99.951	100.051	0.010	>4.1

This Instrument was calibrated using Instruments Traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min = As Left Nominal(Rounded) - Tolerance; Max = As Left Nominal(Rounded) + Tolerance; Date=MM/DD/YY

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Aaron Judice
Aaron Judice, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01
Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-2006-AQ-HOU-RvA.
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).

Item 7

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

- ☒ Model: ALCOTEST CU34
☐ Model: MARK IIA
☐ Other: _____

Serial Number:

DDmKS3-0003

Certification Date:


7-27-17

Technician:

BC

Re-Certification Due Date:

7-27-18



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- ☒ Model: ALCOTEST® CU34
☐ Model: MARK IIA
☐ Other: _____

Serial Number:

DDRKS3-0024

Certification Date

4-26-17

Technician

72

Re-Certification Due Date

4-26-18

Item 8



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

☒ Model: ALCOTEST® CU34

☐ Model: MARK IIA

☐ Other: _____

Serial Number:

DDWES3-0203

Certification Date

3-6-17

Technician

72

Re-Certification Due Date

3-6-18

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications.
For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe: Certification Date: Next Certification Due:

DDHHP2-065

7-13-17

7-13-18

Probe Value:

101

Draeger, Inc.

BC

ITEM 8A

Dräger**Simulator****CERTIFICATE OF ACCURACY**

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

☒ Model: ALCOTEST CU34☐ Model: MARK IIA☐ Other: _____

Serial Number:

DDAN-0041

Certification Date:

10-6-17

Technician:

BC

Re-Certification Due Date:

10-6-18**Dräger****Alcotest 7110 Temperature Probe****CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDXKP2-436

Certification Date:

10-6-17

Next Certification Due:

10-6-18

Probe Value:

103

Dräger, Inc.

BC

ITEM 9

Dräger

Alcotest® 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

5-4-17

SERIAL NUMBER:

ARAJ-0075

Draeger Safety Diagnostics, Inc.

BC

ITEM 10



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

☒ Model: ALCOTEST® CU34

☐ Model: MARK IIA

☐ Other: _____

Serial Number

DDWK53-0386

Certification Date

12-15-16

Technician

VAG

Re-Certification Due Date

12-15-17

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDW3P2-025

Certification date:

12-15-16

Next Certification due:

12-15-17

Probe Value

102

Draeger Safety Diagnostics, Inc.
Technical Service Department

VAG

ITEM 11

Alcotest 7110 Calibration Record

Equipment

Alcotest 7110 MKIII-C
Location: TOMS RIVER P.D.

Serial No.: ARAJ-0075

Calibration File No.: 02147
Certification File No.: 02055
Linearity File No.: 02056
Solution File No.: 02145
Sequential File No.: 02147

Calib. Date: 09/15/2017
Cert. Date: 05/12/2017
Lin. Date: 05/12/2017
Soln. Date: 09/11/2017
File Date: 09/15/2017

Calib. No.: 00029
Cert. No.: 00019
Lin. No.: 00019
Soln. No.: 00251

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 16220

Model No.: CU-34

Serial No.: DDWK S3-0386
Expires: 09/07/2018
Bottle No.: 0428

Coordinator

Last Name: ALCOTT

First Name: KEVIN

MI: W.

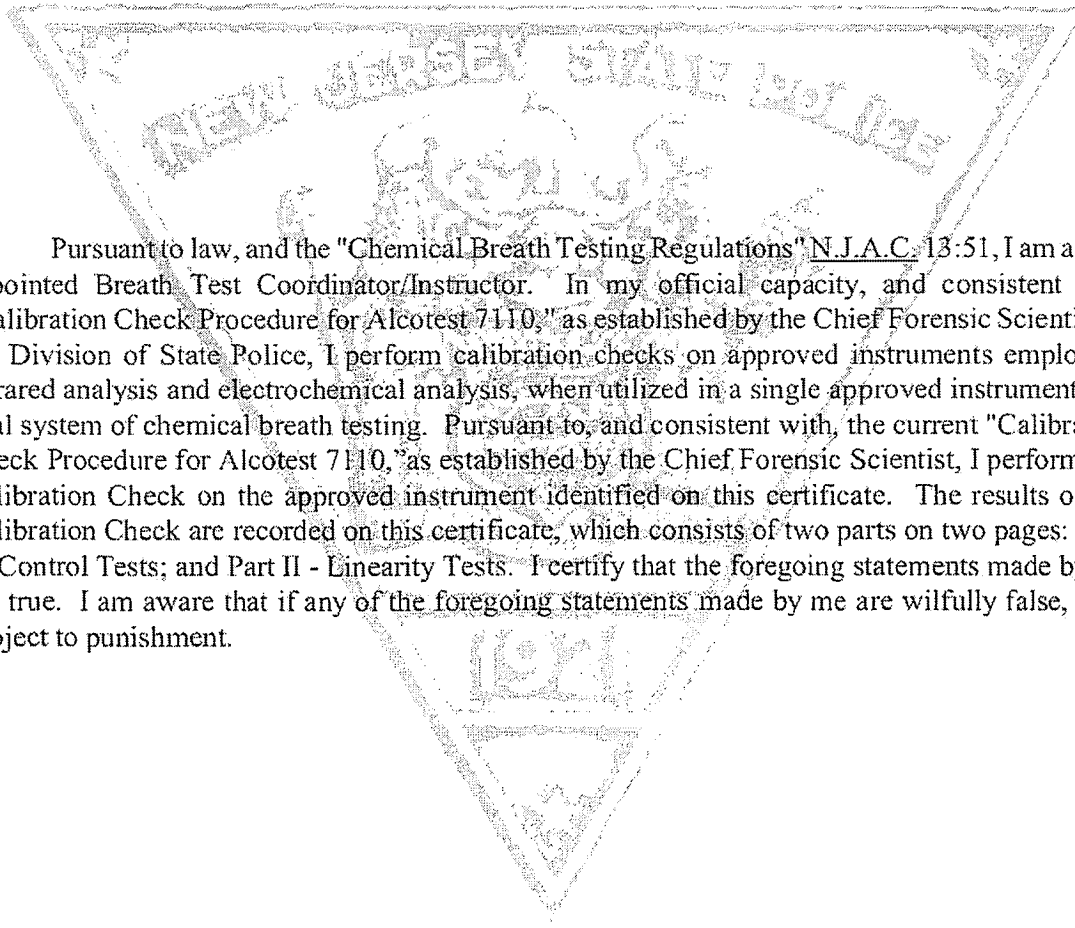
Signature: Tpr. I K W. #6704

Badge No.: 6704

Date: 09/15/2017

*Black Key Temperature Probe Serial.....# DD HHPZ-065 (KA)

*Digital NIST Temperature Measuring System Serial.....# 170 428 368 (KA)



Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Item 12

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment

Alcotest 7110 MKIII-C
Location: TOMS RIVER P.D.
Calibration File No.: 02147
Certification File No.: 02148
Linearity File No.: 02056
Solution File No.: 02145
Sequential File No.: 02148

Serial No.: ARAJ-0075

Calib. Date: 09/15/2017
Cert. Date: 09/15/2017
Lin. Date: 05/12/2017
Soln. Date: 09/11/2017
File Date: 09/15/2017

Calib. No.: 00029
Cert. No.: 00020
Lin. No.: 00019
Soln. No.: 00251

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 16220

Model No.: CU-34

Serial No.: DDWK S3-0386
Expires: 09/07/2018
Bottle No.: 0428

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:31D		
Control 1 EC	0.099%	09:32D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:32D		
Control 2 EC	0.098%	09:33D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:34D		
Control 3 EC	0.098%	09:34D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:35D		

All tests within acceptable tolerance.

Coordinator

Last Name: ALCOTT

First Name: KEVIN

MI: W.

Signature:

Tpt. I K W. Q #6704

Badge No.: 6704

Date: 09/15/2017

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

ITEM 13

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARAJ-0075
Location:	TOMS RIVER P.D.		
Calibration File No.:	02147	Calib. Date:	09/15/2017
Certification File No.:	02148	Cert. Date:	09/15/2017
Linearity File No.:	02149	Lin. Date:	09/15/2017
Solution File No.:	02145	Soln. Date:	09/11/2017
Sequential File No.:	02149	File Date:	09/15/2017
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.040%	Serial No.:	DDMK S3-0003
Solution Control Lot:	16230	Expires:	09/19/2018
		Bottle No.:	0147
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.080%	Serial No.:	DDWE S3-0203
Solution Control Lot:	16250	Expires:	09/27/2018
		Bottle No.:	1442
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.160%	Serial No.:	DDRK S3-0024
Solution Control Lot:	16260	Expires:	10/03/2018
		Bottle No.:	0853

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:53D		
Control 1 EC	0.041%	09:54D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.040%	09:54D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:55D		
Control 2 EC	0.041%	09:56D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.040%	09:56D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:57D		
Control 3 EC	0.081%	09:58D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.081%	09:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:00D		
Control 4 EC	0.081%	10:00D	34.0°C	*** TEST PASSED ***
Control 4 IR	0.079%	10:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:02D		
Control 5 EC	0.162%	10:02D	33.9°C	*** TEST PASSED ***
Control 5 IR	0.160%	10:02D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:04D		
Control 6 EC	0.161%	10:04D	33.9°C	*** TEST PASSED ***
Control 6 IR	0.160%	10:04D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:06D		

All tests within acceptable tolerance.

Coordinator

Last Name: ALCOTT

First Name: KEVIN

MI: W.

Signature: Tr. I K W. Q #6704

Badge No.: 6704

Date: 09/15/2017

ITEM 14

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARAJ-0075
Location:	TOMS RIVER P.D.	
Calibration File No.:	02147	Calib. Date: 09/15/2017
Certification File No.:	02148	Cert. No.: 00029
Linearity File No.:	02149	Cert. Date: 09/15/2017
Solution File No.:	02150	Lin. Date: 09/15/2017
Sequential File No.:	02150	Lin. No.: 00020
		Soln. Date: 09/15/2017
		Soln. No.: 00252
		File Date: 09/15/2017
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWK S3-0386
Solution Control Lot:	17110	Expires: 03/20/2019
		Bottle No.: 0495

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:14D		
Control 1 EC	0.102%	11:15D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:15D		
Control 2 EC	0.101%	11:16D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:17D		
Control 3 EC	0.101%	11:17D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	11:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:18D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDWJPZ-025 (KA)

Changed By:

Last Name: ALCOTT

First Name: KEVIN

MI: W.

Signature: Tr. I NK W. A #6704

Badge No.: 6704

Date: 09/15/2017

ITEM 14A

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARAJ-0075
Location: TOMS RIVER P.D.
Calibration File No.: 02147 Calib. Date: 09/15/2017 Calib. No.: 00029
Certification File No.: 02148 Cert. Date: 09/15/2017 Cert. No.: 00020
Linearity File No.: 02149 Lin. Date: 09/15/2017 Lin. No.: 00020
Solution File No.: 02190 Soln. Date: 11/22/2017 Soln. No.: 00257
Sequential File No.: 02190 File Date: 11/22/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDAN-0041
Control Solution %: 0.100% Expires: 03/20/2019
Solution Control Lot: 17110 Bottle No.: 0099

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:47S		
Control 1 EC	0.100%	08:47S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	08:47S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:48S		
Control 2 EC	0.099%	08:49S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:49S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:49S		
Control 3 EC	0.100%	08:50S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:50S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:51S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: AXKPZ-436 (KA)

Changed By:

Last Name: ALCOTT

First Name: KEVIN

MI: W.

Signature: Tpt. I AK W. Q #6704

Badge No.: 6704

Date: 11/22/2017

ITEM 15



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.


ANALYSIS DATE: 03/29/2017

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 17110

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1211 to 0.1231 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is March 20, 2019.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 30th day of March, 2017.


Notary

MARY ELIZABETH MCLAUGHLIN

ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



Item 16

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Mark S. Nater
Toms River Police Department

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 141 OF THE LAWS OF 1964 IN THE OPERATION OF THE **ALCOTEST 7110 MK III-C**
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, 23th DAY OF December
TWO THOUSAND AND SEVEN

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES 3-28-2005

DATE	Refresher Course PLACE	INSTRUCTOR
1. 11-30-07	Ocean Co. PA	Stank
2. 7-29-09	OCFA	Adam Stank
3. 1-3-11	OCFA	Wm Linn
4. 2-7-13	OCFA	Wm Linn
5. 1-20-15	OCFA	Wm Linn
6. 3-21-17	LAKEHURST	Adam Stank
7.		
8.		
9.		

S.P. 2938 (Rev. 07/07)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Kenneth D. Thomas Jr.
Toms River Township

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 141 OF THE LAWS OF 1964 IN THE OPERATION OF THE **ALCOTEST 7110 MK III-C**
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, 24th DAY OF September
TWO THOUSAND AND NINE

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 1-18-11	OCFA	Wm Linn
2. 1-22-13	OCFA	Wm Linn
3. 2-4-15	OCFA	Wm Linn
4. 4/11/17	LAKEHURST	Adam Stank
5.		
6.		
7.		
8.		
9.		

S.P. 2938 (Rev. 07/07)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Steven Schwartz
Toms River Police Department

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 141 OF THE LAWS OF 1964 IN THE OPERATION OF THE **ALCOTEST 7110 MK III-C**
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, 22nd DAY OF December
TWO THOUSAND AND NINE

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES 1/5/2006

DATE	Refresher Course PLACE	INSTRUCTOR
1. 9/22/2008	Ocean Co.	Cross
2. 1-28-10	OCFA	Wm Linn
3. 2-6-12	OCFA	J. Stank
4. 2-11-14	LAKEHURST	Wm Linn
5. 4-27-16	LAKEHURST	Wm Linn
6.		
7.		
8.		
9.		

S.P. 2938 (Rev. 07/07)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

David Bartoshek
Toms River Township Police Department

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 141 OF THE LAWS OF 1964 IN THE OPERATION OF THE **ALCOTEST 7110 MK III-C**
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, 28th DAY OF February
TWO THOUSAND AND FOURTEEN

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES 1/3/2006

DATE	Refresher Course PLACE	INSTRUCTOR
1. 1/6/2014	Lakehurst	Cross
2. 2-16-16	LAKEHURST	Wm Linn
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2938 (Rev. 08/13)

Item 16-2

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Brian M. Doyle
Toms River Township

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1946 IN THE OPERATION OF THE ALCOTEST 7110 MKIII-C
A METHOD TO DETERMINE INTOXICATION
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 22nd DAY OF October

TWO THOUSAND AND Nine

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

DATE	Refresher Course PLACE	INSTRUCTOR
1. 2-2-11	OCPA	Wm Linn
2. 2-7-13	OCPA	Wm Linn
3. 2-5-15	OCPA	Wm Linn
4. 4/6/17	LAKEHURST	Adam Stankis
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 07/07)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Robert Westfall
Toms River Township Police Department

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1946 IN THE OPERATION OF THE ALCOTEST 7110 MKIII-C
A METHOD TO DETERMINE INTOXICATION
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 24th DAY OF June

TWO THOUSAND AND Ten

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES 1/4/2006

DATE	Refresher Course PLACE	INSTRUCTOR
1. 2/8/2010	Ocean Co. P.A.	Stanks
2. 1/5/11	OCPA	Adam Stankis
3. 1-29-13	OCPA	Wm Linn
4. 3-2-15	OCPA	Wm Linn
5. 4/10/17	LAKEHURST	Adam Stankis
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 03/10)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Michael A. DeRosa
Toms River Township

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1946 IN THE OPERATION OF THE ALCOTEST 7110 MKIII-C
A METHOD TO DETERMINE INTOXICATION
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 4th DAY OF February

TWO THOUSAND AND Fifteen

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES 04/13/2009 - 04/16/2009

DATE	Refresher Course PLACE	INSTRUCTOR
1. 02/11/2014	Lakehurst	CROSS
2. 2-17-16	LAKEHURST	Wm Linn
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 08/13)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Adam M. Koeppe
Toms River Township

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1946 IN THE OPERATION OF THE ALCOTEST 7110 MKIII-C
A METHOD TO DETERMINE INTOXICATION
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 21st DAY OF March

TWO THOUSAND AND Eleven

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 1/17/13	OCPA	Adam Stankis
2. 1-22-15	OCPA	Wm Linn
3. 4/26/17	LAKEHURST	Adam Stankis
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 03/10)

Item 16-3

DEPARTMENT OF
Water and Public Safety
This is to certify that

Pascal M. Gambardella, Jr.
Toms River Township

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 143 OF
THE LAWS OF 1944 IN THE OPERATION OF THE Alcotest 7110 MKIII-C
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 7th DAY OF March

TWO THOUSAND AND Thirteen

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. <u>3/3/15</u>	<u>OC.PA</u>	<u>Adam Standa</u>
2. <u>4/27/17</u>	<u>LAKEHURST</u>	<u>Adam Standa</u>
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 293B (Rev. 02/12)

DEPARTMENT OF
Water and Public Safety
This is to certify that

Ronald C. Bayer
Toms River Township

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 143 OF
THE LAWS OF 1944 IN THE OPERATION OF THE Alcotest 7110 MKIII-C
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 5th DAY OF April

TWO THOUSAND AND Twelve

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. <u>1-23-14</u>	<u>LAKEHURST</u>	<u>Wm. Lynn</u>
2. <u>4-21-16</u>	<u>LAKEHURST</u>	<u>Wm. Lynn</u>
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 293B (Rev. 02/12)