

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWF-0394
Location: TOMS RIVER P.D.
Calibration File No.: 01682 Calib. Date: 07/18/2018 Calib. No.: 00040
Certification File No.: 01683 Cert. Date: 07/18/2018 Cert. No.: 00030
Linearity File No.: 01684 Lin. Date: 07/18/2018 Lin. No.: 00030
Solution File No.: 01688 Soln. Date: 08/10/2018 Soln. No.: 00264
Sequential File No.: 01688 File Date: 08/10/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWK S3-0387
Control Solution %: 0.100% Expires: 12/11/2019
Solution Control Lot: 17420 Bottle No.: 1152

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 12:37D | | |
| Control 1 EC | 0.101% | 12:37D | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.100% | 12:37D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 12:38D | | |
| Control 2 EC | 0.099% | 12:39D | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.097% | 12:39D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 12:39D | | |
| Control 3 EC | 0.098% | 12:40D | 34.0°C | CONTROL TEST FAILED |
| Control 3 IR | 0.094% | 12:40D | 34.0°C | CONTROL TEST FAILED |
| Ambient Air Blank | 0.000% | 12:41D | | |

Test results are not within acceptable range.

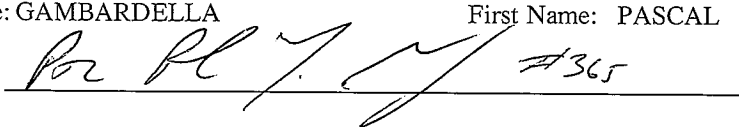
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: GAMBARDELLA

First Name: PASCAL

MI: M

Signature:  #365

Badge No.: 365

Date: 08/10/2018