

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARAJ-0075
Location: TOMS RIVER P.D.
Calibration File No.: 02397 Calib. Date: 07/18/2018 Calib. No.: 00031
Certification File No.: 02398 Cert. Date: 07/18/2018 Cert. No.: 00022
Linearity File No.: 02399 Lin. Date: 07/18/2018 Lin. No.: 00022
Solution File No.: 02500 Soln. Date: 11/21/2018 Soln. No.: 00292
Sequential File No.: 02500 File Date: 11/21/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWK S3-0386
Control Solution %: 0.100% Expires: 12/11/2019
Solution Control Lot: 17420 Bottle No.: 1169

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:03S		
Control 1 EC	0.102%	12:03S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:04S		
Control 2 EC	0.099%	12:05S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	12:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:05S		
Control 3 EC	0.100%	12:06S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	12:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:07S		

All tests within acceptable tolerance.

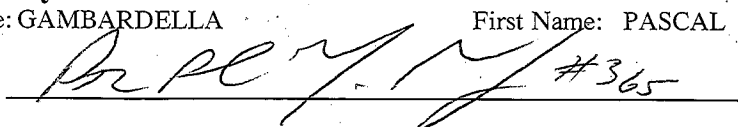
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: GAMBARDELLA

First Name: PASCAL

MI: M

Signature:  #365

Badge No.: 365

Date: 11/21/2018