

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARWF-0394  
Location: TOMS RIVER P.D.  
Calibration File No.: 01891 Calib. Date: 02/12/2021 Calib. No.: 00051  
Certification File No.: 01892 Cert. Date: 02/12/2021 Cert. No.: 00038  
Linearity File No.: 01893 Lin. Date: 02/12/2021 Lin. No.: 00038  
Solution File No.: 01913 Soln. Date: 04/23/2021 Soln. No.: 00322  
Sequential File No.: 01913 File Date: 04/23/2021

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDAN-0040  
Control Solution %: 0.100% Expires: 01/13/2023  
Solution Control Lot: 21010 Bottle No.: 0095

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:21D		
Control 1 EC	0.100%	11:22D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:22D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:22D		
Control 2 EC	0.098%	11:23D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:23D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:24D		
Control 3 EC	0.098%	11:24D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:24D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:25D		

All tests within acceptable tolerance.

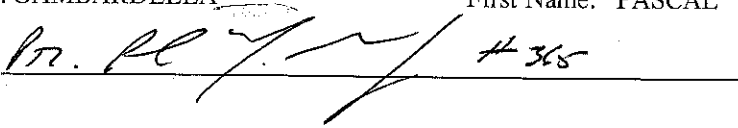
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

## Changed By:

Last Name: GAMBARDELLA

First Name: PASCAL

MI: M

Signature: 

Badge No.: 365

Date: 04/23/2021