

Calibrating Unit New Standard Solution Report

| | | | |
|-------------------------|-----------------------|--------------|--------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: | ARAJ-0075 |
| Location: | TOMS RIVER P.D. | Calib. Date: | 06/23/2021 |
| Calibration File No.: | 03094 | Calib. No.: | 00043 |
| Certification File No.: | 03095 | Cert. Date: | 06/23/2021 |
| Linearity File No.: | 03096 | Cert. No.: | 00030 |
| Solution File No.: | 03233 | Lin. Date: | 06/23/2021 |
| Sequential File No.: | 03233 | Lin. No.: | 00030 |
| | | Soln. Date: | 11/27/2021 |
| | | Soln. No.: | 00412 |
| | | File Date: | 11/27/2021 |
| | | | |
| Calibrating Unit: | WET | Model No.: | CU-34 |
| Control Solution %: | 0.100% | Serial No.: | DDWK S3-0386 |
| Solution Control Lot: | 21150 | Expires: | 05/04/2023 |
| | | Bottle No.: | 0683 |

| Function | Result %BAC | Time HH:MM | Temperature Simulator (°C) | Comment(s) or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000% | 01:49S | | |
| Control 1 EC | 0.099% | 01:49S | 33.9°C | *** TEST PASSED *** |
| Control 1 IR | 0.100% | 01:49S | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 01:50S | | |
| Control 2 EC | 0.098% | 01:51S | 33.9°C | *** TEST PASSED *** |
| Control 2 IR | 0.100% | 01:51S | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 01:51S | | |
| Control 3 EC | 0.097% | 01:52S | 33.9°C | *** TEST PASSED *** |
| Control 3 IR | 0.099% | 01:52S | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 01:53S | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CASO

First Name: JARED

MI: J

Signature: _____

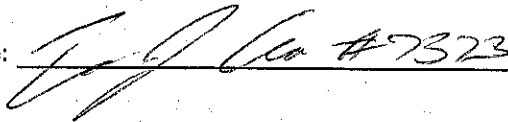

Badge No.: 7373

Date: 11/27/2021