

ALCOTEST CERTIFICATIONS INDEX # 35
07-26-2023

ARAJ-0075

- ITEM # 1 - NJSP OFFICER'S ALCOTEST CREDENTIALS
- ITEM # 2 - CERT OF ANALYSIS SIMULATOR SOLUTION 0.10
- ITEM # 3 - CERT OF ANALYSIS SIMULATOR SOLUTION 0.04
- ITEM # 4 - CERT OF ANALYSIS SIMULATOR SOLUTION 0.08
- ITEM # 5 - CERT OF ANALYSIS SIMULATOR SOLUTION 0.16
- ITEM # 6 - NIST CERT (2 PGS)
- ITEM # 7 - ALCOTEST CU34 SERIAL #DDSCS3-0005
- ALCOTEST CU34 SERIAL #DDWES3-2011
- ITEM # 8 - ALCOTEST CU34 SERIAL #DDXCS3-0020
- ALCOTEST TEMPERATURE PROBE SERIAL # DDEEP2-060
- ITEM # 9 - TRPD ALCOTEST 7110 MK111-C SERIAL # ARAJ-0075
- ITEM # 10 - TRPD ALCOTEST CU34 SERIAL # DDAN-0041
- TRPD ALCOTEST TEMP PROBE SERIAL # DDXKP2-436
- ITEM # 11 - ALCOTEST 7110 MKIII-C DIGITAL THERMOMETER READINGS
- ITEM # 12 - ALCOTEST 7110 CALIBRATION RECORD
- ITEM # 13 - ALCOTEST 7110 CALIBRATION CONTROL TESTS
- ITEM # 14 - ALCOTEST 7110 CALIBRATION LINEARITY TESTS
- ITEM # 15 - NJSP NEW STANDARD SOLUTION REPORT 500
- ITEM # 16 - CERTIFICATE OF ANALYSIS SIMULATOR SOLUTION (23010)
- ITEM # 17 - ALCOTEST CARDS/SOLUTION CHANGE OPERATOR (3PGS.)

ITHm-2



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

MATTHEW J. PLATKIN
Acting Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS 0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 07/21/2022

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 22240

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1205 to 0.1219 grams per 100 milliliters of solution.


This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 05, 2024.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 27 day of July, 2022.

[Signature]
Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

MATTHEW J. PLATKIN
Acting Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS 0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 08/17/2022

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 22250

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0479 to 0.0483 grams per 100 milliliters of solution.


This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 19, 2024.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 9 day of September, 2022.

Notary

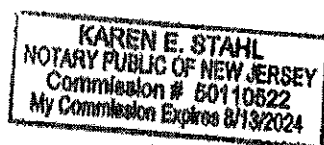

"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



Item-4



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 832-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

MATTHEW J. PLATKIN
Acting Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS 0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.


ANALYSIS DATE: 08/18/2022


BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 22270

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0967 to 0.0983 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 28, 2024.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 9 day of September, 2022.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110822
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



ITEM-5



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

MATTHEW J. PLATKIN
Acting Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS 0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.


ANALYSIS DATE: 08/22/2022

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 22290

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1924 to 0.1948 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 4, 2024.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 9 day of September, 2022.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001

Cert. No.: 4000-13326294



Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by : VWR International LLC Radnor Corporate Center, Bldg 1, Ste 200, 100 Malsonford Road, Radnor, PA, 19087

Instrument Identification:

Model: 61220-601,

S/N: 221473033

Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath	93139		
Temperature Probe	128	09 Jul 2022	15-D4F0Q-40-1
Thermistor Module	A17118	08 Jul 2022	1000469276
Temperature Calibration Bath	A45240		
Temperature Calibration Bath	A42238		
Temperature Calibration Bath	B01375		
Thermistor Module	B96381	18 Aug 2022	1000470702
Temperature Probe	5392	04 Aug 2022	4500006080
Temperature Probe	5398	24 Aug 2022	4500006081
Thermistor Module	B96382	08 Oct 2022	1000472708
Temperature Probe	5410	20 Oct 2022	4500006780

Certificate Information:

Technician: 299

Procedure: CAL-06

Cal Date: 25 Apr 2022

Cal Due Date: 25 Apr 2024

Test Conditions: 58.46%RH 23.43°C 1017mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C	N.A.	N.A.		0.000	0.001	Y	-0.05	0.05	0.0087	>4:1
°C	N.A.	N.A.		25.000	25.001	Y	24.95	25.05	0.0087	>4:1
°C	N.A.	N.A.		50.000	50.001	Y	49.95	50.05	0.0087	>4:1
°C	N.A.	N.A.		100.000	100.003	Y	99.95	100.05	0.0087	>4:1

This certificate indicates Traceability to standards provided by (NIST) National Institute of Standards and Technology and/or a National Standards Laboratory.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO Guide to the Expression of Uncertainty in Measurement (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min=As Left Nominal(Rounded) - Tolerance; Max=As Left Nominal(Rounded) + Tolerance;

Nicol Rodriguez

Nicol Rodriguez, Quality Manager

Marisa Elms

Marisa Elms, Technical Manager

Note :

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometer change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com

Control Company is an ISO/IEC 17025:2017 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1760.01.
Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-ANAB.
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001

Cert. No.: 4000-13326294



Traceable® Certificate of Calibration for Digital Thermometer

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

Issue Date : 25 Apr 2022

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com

Control Company is an ISO/IEC 17025:2017 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-ANAB.
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).

Item 7

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

☒ Model: ALCOTEST CU34

☐ Model: MARK IIA

☐ X-Cal 2000 (Alcosim)

☐ Other: _____

Serial Number:

DDSCS3-0005

Certification Date:

5-22-23

Technician:

DH / MB

Re-Certification Due Date:

5-22-24

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

☒ Model: ALCOTEST CU34

☐ Model: MARK IIA

☐ X-Cal 2000 (Alcosim)

☐ Other: _____

Serial Number:

DDWES3-0211

Certification Date:

5-22-23

Technician:

DH / MB

Re-Certification Due Date:

5-22-24

ITEM 8

Dräger**Simulator****CERTIFICATE OF ACCURACY**

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

☒ Model: ALCOTEST CU34☐ Model: MARK IIA☐ X-Cal 2000 (Alcosim)☐ Other: _____

Serial Number:

DDXCS3-0020

Certification Date:

5-22-23

Technician:

DH / MB

Re-Certification Due Date:

5-22-24**Dräger****Alcotest 7110 Temperature Probe****CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDEE P2-060

Certification Date:

5-30-23

Next Certification Due:


5-30-24

Probe Value:

106

Draeger, Inc.

DH / MB

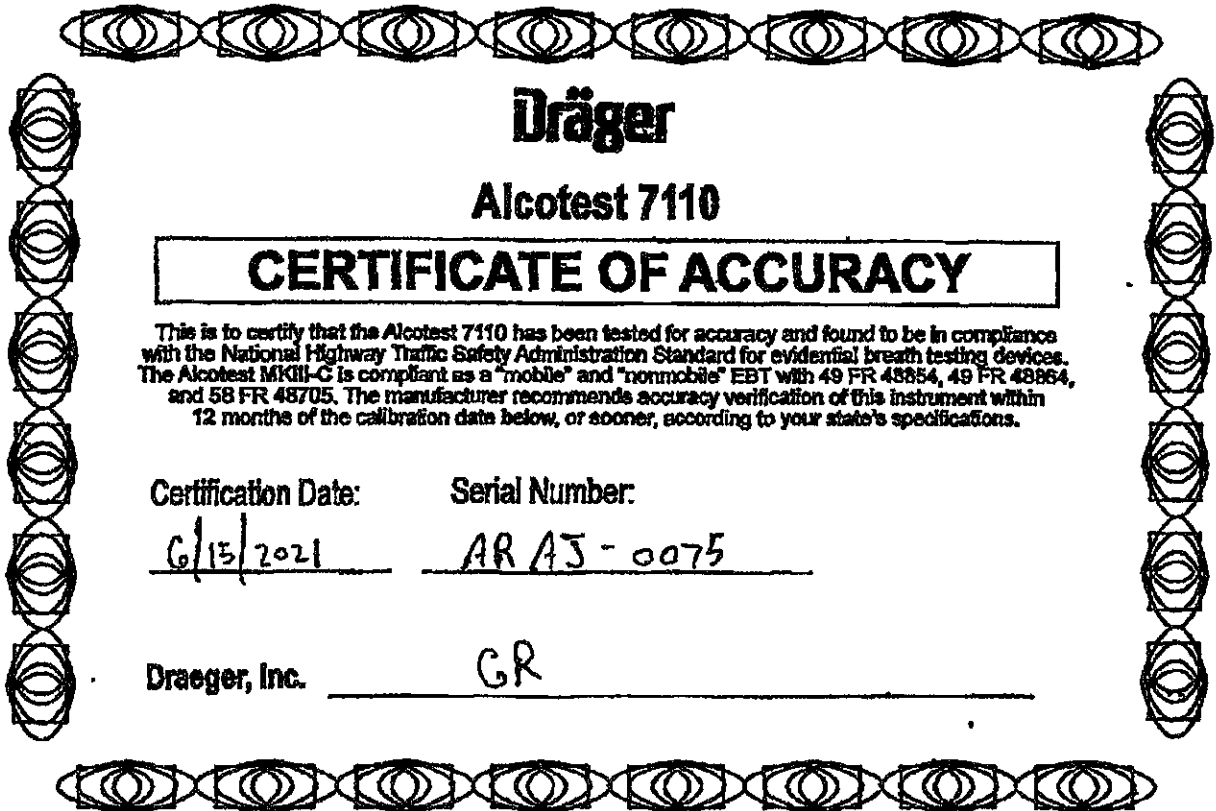

Dräger

Alcotest 7110

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-G is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864, and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your state's specifications.

Certification Date: 6/15/2021 Serial Number: AR 45 - 0075

Dräger, Inc. GR

Dräger**Simulator****CERTIFICATE OF ACCURACY**

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger, Inc.

- ☒ Model: ALCOTEST CU34
☐ Model: MARK IIA
☐ X-Cal 2000 (Alcosim)
☐ Other: _____

Serial Number:

DDAN-0041

Certification Date:

11-21-22

Technician:

MB/DH

Re-Certification Due Date:

11-21-23**Dräger****Alcotest 7110 Temperature Probe****CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDX KP2-436

Certification Date:

11-21-22

Next Certification Due:

11-21-23

Probe Value:

106

Draeger, Inc.

MB/DH

Alcotest 7110 MKIII-C Calibration **NIST-Traceable Digital Thermometer Readings**

Coordinator:

Tpr I Dennis J Lutz
 Name

7045
 Badge No.

Location:

Toms River P.D.
 Agency

ARAJ-0075
 Alcotest Serial No.

Equipment:

221 473 033
 Digital NIST Temperature Measuring System Serial No.

Simulator Solution Concentration	CU-34 Simulator Serial No.	Time Simulators Started to Heat	Time Temp. Reading Obtained	Temp. Reading on NIST Traceable Thermometer
0.04%	DDSC S3- 0005	08:00 D	09:05 D	33.9°C
0.08%	DDWE S3- 0211	08:00 D	09:06 D	33.9°C
0.10%	DDAN- 0041	08:00 D	09:07 D	34.0°C
0.16%	DDXC S3- 0020	08:00 D	09:08 D	33.9°C

Pursuant to law and the "Chemical Breath Testing Regulations" established at N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity and consistent with the "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on Alcotest 7110 MKIII-C instruments. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110", I performed a Calibration Check Procedure on the Alcotest 7110 MKIII-C instrument identified on this certificate. Pursuant to the current "Calibration Check Procedure for Alcotest 7110", I used the Digital NIST-traceable Temperature Measuring System identified on this certificate to confirm that the temperatures of the 0.10%, 0.04%, 0.08%, and 0.16% Simulator Solutions used in the respective CU-34 Simulators identified on this certificate, were 34.0 degrees Celsius $\pm$ 0.2 degrees Celsius. I hereby certify that I truthfully recorded on this certificate the temperatures of each of the simulator solutions as shown on the Digital NIST-traceable Temperature Measuring System thermometer. I am aware that if any of the foregoing statements made by me are willfully false, I am subject to punishment.

Tpr I [Signature] 7045
 Coordinator's Signature

7-26-23
 Date

Alcotest 7110 Calibration Record

Equipment

Alcotest 7110 MKIII-C
Location: TOMS RIVER P.D.

Serial No.: ARAJ-0075

Calibration File No.: 03704
Certification File No.: 03607
Linearity File No.: 03608
Solution File No.: 03703
Sequential File No.: 03704

Calib. Date: 07/26/2023
Cert. Date: 03/20/2023
Lin. Date: 03/20/2023
Soln. Date: 07/10/2023
File Date: 07/26/2023

Calib. No.: 00048
Cert. No.: 00034
Lin. No.: 00034
Soln. No.: 00499

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 22240

Model No.: CU-34

Serial No.: DDAN-0041
Expires: 07/05/2024
Bottle No.: 0888

Coordinator

Last Name: LUTZ

First Name: DENNIS


MI: J

Signature: Tpr I Lutz 7045

Badge No.: 7045

Date: 07/26/2023

*Black Key Temperature Probe Serial.....# DDEE P2-066 (DL)
*Digital NIST Temperature Measuring System Serial.....# 221 473 033 (DL)

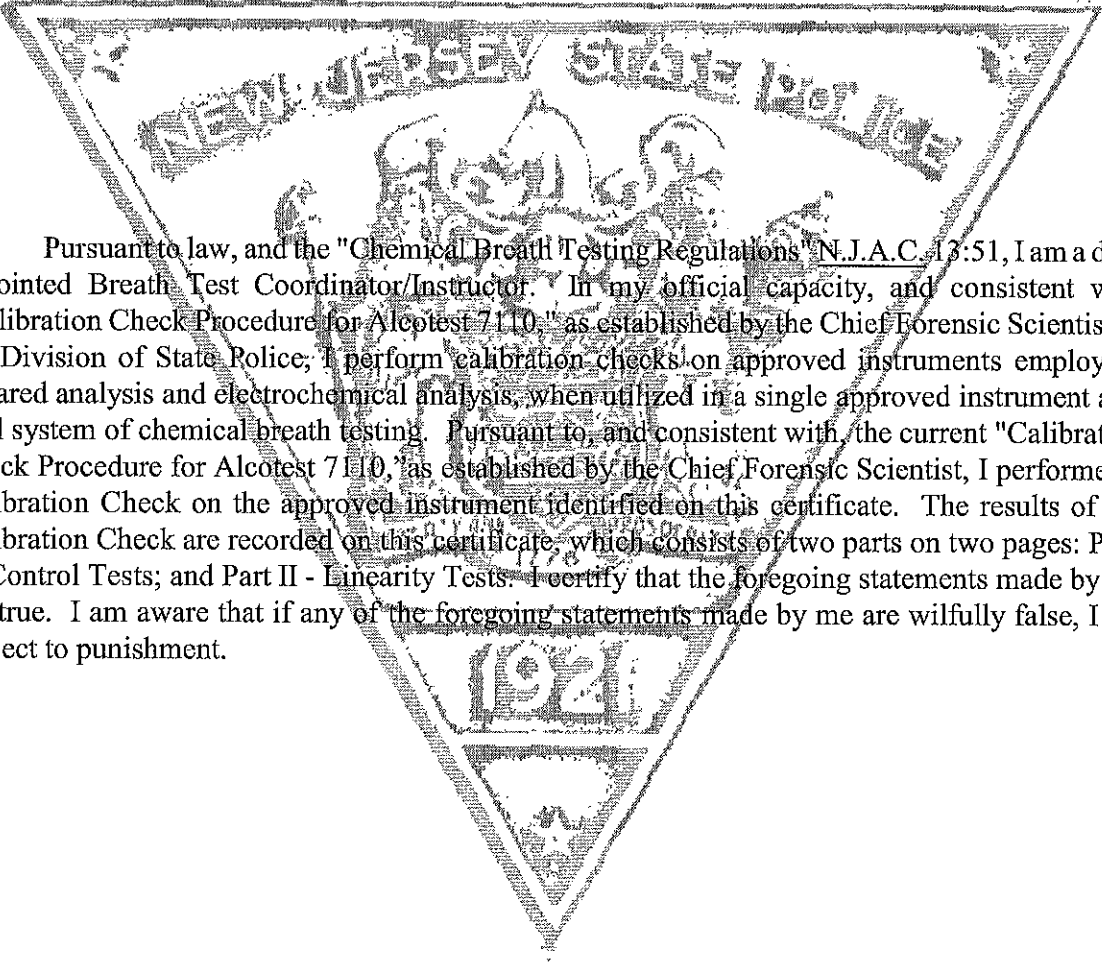

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 17:27, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARAJ-0075
Location:	TOMS RIVER P.D.	
Calibration File No.:	03704	Calib. Date: 07/26/2023
Certification File No.:	03705	Calib. No.: 00048
Linearity File No.:	03608	Cert. Date: 07/26/2023
Solution File No.:	03703	Cert. No.: 00035
Sequential File No.:	03705	Lin. Date: 03/20/2023
		Lin. No.: 00034
		Soln. Date: 07/10/2023
		Soln. No.: 00499
		File Date: 07/26/2023
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDAN-0041
Solution Control Lot:	22240	Expires: 07/05/2024
		Bottle No.: 0888

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:19D		
Control 1 EC	0.099%	09:20D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:20D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:20D		
Control 2 EC	0.097%	09:21D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	09:21D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:22D		
Control 3 EC	0.099%	09:22D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:22D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:23D		

All tests within acceptable tolerance.

Coordinator

Last Name: LUTZ

First Name: DENNIS

MI: J

Signature: _____

Badge No.: 7045

Date: 07/26/2023

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARAJ-0075
Location:	TOMS RIVER P.D.		
Calibration File No.:	03704	Calib. Date:	07/26/2023
Certification File No.:	03705	Cert. Date:	07/26/2023
Linearity File No.:	03706	Lin. Date:	07/26/2023
Solution File No.:	03703	Soln. Date:	07/10/2023
Sequential File No.:	03706	File Date:	07/26/2023
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.040%	Serial No.:	DDSC S3-0005
Solution Control Lot:	22250	Expires:	07/19/2024
		Bottle No.:	1361
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.080%	Serial No.:	DDWE S3-0211
Solution Control Lot:	22270	Expires:	07/28/2024
		Bottle No.:	0192
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.160%	Serial No.:	DDXC S3-0020
Solution Control Lot:	22290	Expires:	08/04/2024
		Bottle No.:	0405

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:38D		
Control 1 EC	0.042%	09:38D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.041%	09:38D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:40D		
Control 2 EC	0.041%	09:40D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.041%	09:40D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:42D		
Control 3 EC	0.082%	09:42D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.079%	09:42D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:44D		
Control 4 EC	0.080%	09:44D	33.9°C	*** TEST PASSED ***
Control 4 IR	0.080%	09:44D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:46D		
Control 5 EC	0.165%	09:46D	33.9°C	*** TEST PASSED ***
Control 5 IR	0.160%	09:46D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:48D		
Control 6 EC	0.162%	09:48D	33.9°C	*** TEST PASSED ***
Control 6 IR	0.160%	09:48D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:50D		

All tests within acceptable tolerance.

Coordinator

Last Name: LUTZ

First Name: DENNIS

MI: J

Signature: _____

Badge No.: 7045

Date: 07/26/2023

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARAJ-0075
Location:	TOMS RIVER P.D.		
Calibration File No.:	03704	Calib. Date:	07/26/2023
Certification File No.:	03705	Cert. No.:	00035
Linearity File No.:	03706	Lin. Date:	07/26/2023
Solution File No.:	03707	Soln. Date:	07/26/2023
Sequential File No.:	03707	File Date:	07/26/2023
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDAN-0041
Solution Control Lot:	23010	Expires:	01/11/2025
		Bottle No.:	0846

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:04D		
Control 1 EC	0.103%	11:05D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.103%	11:05D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:06D		
Control 2 EC	0.101%	11:06D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.103%	11:06D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:07D		
Control 3 EC	0.101%	11:07D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.103%	11:07D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:08D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number:

DDXKP2-436

(DC)

Changed By:

Last Name: LUTZ

First Name: DENNIS

MI: J

Signature:

[Handwritten Signature] 7045

Badge No.: 7045

Date: 07/26/2023



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

MATTHEW J. PLATKIN
Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS 0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 01/25/2023

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 23010

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1211 to 0.1225 grams per 100 milliliters of solution.


This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 11, 2025.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 30 day of January, 2023.

Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



DEPARTMENT OF
Water and Public Safety
This is to certify that

Ronald C. Bayer
Toms River Township

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1964 IN THE OPERATION OF THE ALCOTEST 7110 MK III-C
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 5th DAY OF April

TWO THOUSAND AND Twelve
SUPERINTENDENT
NEW JERSEY STATE POLICE

ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 1-23-14	LAKEHURST	Wm Cross
2. 4-21-16	LAKEHURST	Wm Cross
3. 3-27-18	LAKEHURST	Adam Stankis
4. 8-16-20	ALLC	Adam Stankis
5. 9-17-22	Lakehurst	JAH
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 02/12)

DEPARTMENT OF
Water and Public Safety
This is to certify that

Steven Schwartz
Toms River Police Department

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1964 IN THE OPERATION OF THE ALCOTEST 7110 MK III-C
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 22nd DAY OF December

TWO THOUSAND AND Nine
SUPERINTENDENT
NEW JERSEY STATE POLICE

ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

1/3/2006

DATE	Refresher Course PLACE	INSTRUCTOR
1. 9/22/2008	Ocean Co.	Cross
2. 1-28-10	OCPA	Wm Cross
3. 2-6-12	OCPA	J. Schryver
4. 2-11-14	LAKEHURST	Wm Cross
5. 4-27-16	LAKEHURST	Wm Cross
6. 8-16-18	ALLC	Adam Stankis
7. 8-13-20	ALLC	Adam Stankis
8. 9-18-22	Lakehurst	Brunn
9.		

S.P. 293B (Rev. 07/07)

DEPARTMENT OF
Water and Public Safety
This is to certify that

Robert Westfall
Toms River Township Police Department

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1964 IN THE OPERATION OF THE ALCOTEST 7110 MK III-C
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 14th DAY OF June

TWO THOUSAND AND Ten
SUPERINTENDENT
NEW JERSEY STATE POLICE

ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

1/4/2006

DATE	Refresher Course PLACE	INSTRUCTOR
1. 2/8/2010	Ocean Co. P.A.	Stanks
2. 1/5/11	OCPA	Adam Stankis
3. 1-29-13	OCPA	Wm Cross
4. 3-2-15	OCPA	Wm Cross
5. 4-10-17	LAKEHURST	Adam Stankis
6. 5-29-19	LAKEHURST	Wm Cross
7. 8-12-21	Lakehurst	R. A.
8. 3-1-23	Lakehurst	JAH
9.		

S.P. 293B (Rev. 03/10)

DEPARTMENT OF
Water and Public Safety
This is to certify that

David Bartoshek
Toms River Township Police Department

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1964 IN THE OPERATION OF THE ALCOTEST 7110 MK III-C
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 28th DAY OF February

TWO THOUSAND AND Fourteen
SUPERINTENDENT
NEW JERSEY STATE POLICE

ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

1/3/2006

DATE	Refresher Course PLACE	INSTRUCTOR
1. 1/6/2014	Lakehurst	Cross
2. 2-16-16	LAKEHURST	Wm Cross
3. 3-27-18	LAKEHURST	Wm Cross
4. 8-14-20	ALLC	Adam Stankis
5. 4-19-22	Lakehurst	JAH
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 08/13)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Matthew S. Natter
Toms River Police Department
IS QUALIFIED AND COMPETENT TO CONDUCT CHLORIDE BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1966 IN THE OPERATION OF THE ALCOHOL TEST 7110 MK III-C
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 14th DAY OF December
TWO THOUSAND AND SEVEN

[Signature] SUPERINTENDENT
[Signature] ATTORNEY GENERAL
NEW JERSEY STATE POLICE

ORIGINAL COURSE DATES 3-28-2005

DATE	Refresher Course PLACE	INSTRUCTOR
1. 11-30-07	Ocean Co. PA	Stanks
2. 7-29-09	OCPA	Adam Stankis
3. 1-3-11	OCPA	Wm Hoss
4. 2-7-13	OCPA	Wm Hoss
5. 1-20-15	OCPA	Wm Hoss
6. 3-21-17	LAKEHURST	Adam Stankis
7. 4-15-19	LAKEHURST	Wm Hoss
8. 7-7-21	Lakehurst	Ha Duong
9.		

S.P. 293B (Rev. 07/07)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Adam M. Koeppe
Toms River Police Department
IS QUALIFIED AND COMPETENT TO CONDUCT CHLORIDE BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1966 IN THE OPERATION OF THE ALCOHOL TEST 7110 MK III-C
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 11th DAY OF March
TWO THOUSAND AND ELEVEN

[Signature] SUPERINTENDENT
[Signature] ATTORNEY GENERAL
NEW JERSEY STATE POLICE

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 1/17/13	OCPA	Adam Stankis
2. 1-22-15	OCPA	Wm Hoss
3. 4/26/17	LAKEHURST	Adam Stankis
4. 1-24-19	Lakehurst	R. G.
5. 8-5-21	Lakehurst	Wm Hoss
6. 3/24/23	Lakehurst	Ha Duong
7.		
8.		
9.		

S.P. 293B (Rev. 03/10)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Pascal M. Gambardella, Jr.
Toms River Township
IS QUALIFIED AND COMPETENT TO CONDUCT CHLORIDE BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1966 IN THE OPERATION OF THE ALCOHOL TEST 7110 MK III-C
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 7th DAY OF March
TWO THOUSAND AND THIRTEEN

[Signature] SUPERINTENDENT
[Signature] ATTORNEY GENERAL
NEW JERSEY STATE POLICE

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 3/3/15	OCPA	Adam Stankis
2. 4/27/17	LAKEHURST	Adam Stankis
3. 5/9/19	LAKEHURST	Adam Stankis
4. 7-9-21	Lakehurst	Ha Duong
5. 3/3/23	Lakehurst	Ha Duong
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 03/10)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Michael P. Cassidy Jr.
Toms River Township
IS QUALIFIED AND COMPETENT TO CONDUCT CHLORIDE BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1966 IN THE OPERATION OF THE ALCOHOL TEST 7110 MK III-C
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 23rd DAY OF May
TWO THOUSAND AND SIXTEEN

[Signature] SUPERINTENDENT
[Signature] ATTORNEY GENERAL
NEW JERSEY STATE POLICE

ORIGINAL COURSE DATES 08/26/2013 - 08/29/2013

DATE	Refresher Course PLACE	INSTRUCTOR
1. 02/03/2015	Ocean Co. P.A.	Stanks
2. 4-5-17	LAKEHURST	Wm Hoss
3. 4/16/19	LAKEHURST	Adam Stankis
4. 7/20/21	Lakehurst	Ha Duong
5. 3/8/23	Lakehurst	Ha Duong
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 03/13)

DEPARTMENT OF
Health and Public Safety
 This is to certify that

Ryan P. Fitzgerald
 Toms River Township

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
 THE LAWS OF 1966 IN THE OPERATION OF THE **Alcotest 7110 MKIII-C**
 A METHOD TO DETERMINE INTOXICATION
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 25th DAY OF May

TWO THOUSAND AND Seventeen

[Signature]
 SUPERINTENDENT
 NEW JERSEY STATE POLICE

[Signature]
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. <u>5/9/19</u>	<u>LAKEHURST</u>	<u>Adam Standa</u>
2. <u>8-3-21</u>	<u>Lakehurst</u>	<u>Halley</u>
3. <u>2/28/23</u>	<u>Lakehurst</u>	<u>B...</u>
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 08/16)

DEPARTMENT OF
Health and Public Safety
 This is to certify that

John R. Marsicano
 Toms River Township

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
 THE LAWS OF 1966 IN THE OPERATION OF THE **Alcotest 7110 MKIII-C**
 A METHOD TO DETERMINE INTOXICATION
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 15th DAY OF February

TWO THOUSAND AND 18

[Signature]
 SUPERINTENDENT
 NEW JERSEY STATE POLICE

[Signature]
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. <u>8/13/20</u>	<u>ALL</u>	<u>Adam Standa</u>
2. <u>4/21/22</u>	<u>Lakehurst</u>	<u>Halley</u>
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 03/19)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Ronald C. Bayer
Toms River Township

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1964 IN THE OPERATION OF THIS ALCOTEST 7110 MKIII-C
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 5th DAY OF April

TWO THOUSAND AND Twelve

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 1-23-14	LAKEHURST	Wm Linn
2. 4-21-16	LAKEHURST	Wm Linn
3. 3-27-18	LAKEHURST	Adam Stankin
4. 8-6-20	ALLC	Adam Stankin
5. 9-7-22	Lakehurst	JS/LL
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 02/12)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Steven Schwartz
Toms River Police Department

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1964 IN THE OPERATION OF THIS ALCOTEST 7110 MK III-C
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 22nd DAY OF December

TWO THOUSAND AND Nine

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

1/5/2006

DATE	Refresher Course PLACE	INSTRUCTOR
1. 9/22/2008	Ocean Co.	Cross
2. 1-28-10	OCPA	Wm Linn
3. 2-6-12	OCPA	J. Smyth
4. 2-11-14	LAKEHURST	Wm Linn
5. 4-27-16	LAKEHURST	Wm Linn
6. 8-16-18	NJSP. Lakehurst	Adam Stankin
7. 8-13-20	ALLC	Adam Stankin
8. 9-18-22	Lakehurst	Brum
9.		

S.P. 293B (Rev. 07/07)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Robert Westfall
Toms River Township Police Department

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1964 IN THE OPERATION OF THIS ALCOTEST 7110 MKIII-C
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 14th DAY OF June

TWO THOUSAND AND Ten

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

1/4/2006

DATE	Refresher Course PLACE	INSTRUCTOR
1. 2/8/2010	Ocean Co. P.A.	Stanks
2. 1/5/11	OCPA	Adam Stankin
3. 1-29-13	OCPA	Wm Linn
4. 3-2-15	OCPA	Wm Linn
5. 4/10/17	LAKEHURST	Adam Stankin
6. 5-29-19	LAKEHURST	Wm Linn
7. 8/2/21	Lakehurst	AK 9
8. 3/1/23	Lakehurst	JS/LL
9.		

S.P. 293B (Rev. 03/10)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

David Bartoshek
Toms River Township Police Department

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1964 IN THE OPERATION OF THIS ALCOTEST 7110 MK III-C
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 28th DAY OF February

TWO THOUSAND AND Fourteen

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

1/3/2006

DATE	Refresher Course PLACE	INSTRUCTOR
1. 1/6/2014	Lakehurst	Cross
2. 2-16-16	LAKEHURST	Wm Linn
3. 3-27-18	LAKEHURST	Wm Linn
4. 8/4/20	ALLC	Adam Stankin
5. 4/19/22	Lakehurst	JS/LL
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 08/13)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Mark S. Natter
Toms River Police Department
IS QUALIFIED AND COMPETENT TO CONDUCT CHIMIC BREATH ANALYSES PURSUANT TO CHAPTER 143 OF
THE LAWS OF 1966 IN THE OPERATION OF THE ALCOHOL TEST 7110 MK III-C
A METHOD TO DETERMINE INTOXICATION
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, this 15th DAY OF December
TWO THOUSAND AND SEVEN

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES 3-28-2005

DATE	Refresher Course PLACE	INSTRUCTOR
1. 11-30-07	Ocean Co. PA	Stanks
2. 7-29-09	OCPA	Adam Stankis
3. 1-3-11	OCPA	Wm. Ross
4. 2-7-13	OCPA	Wm. Ross
5. 1-20-15	OCPA	Wm. Ross
6. 3-21-17	LAKEHURST	Adam Stankis
7. 4-15-19	LAKEHURST	Wm. Ross
8. 7-7-21	Lakehurst	Hal Dulay
9.		
10.		

S.P. 293B (Rev. 07/07)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Adam M. Koopen
Toms River Township
IS QUALIFIED AND COMPETENT TO CONDUCT CHIMIC BREATH ANALYSES PURSUANT TO CHAPTER 143 OF
THE LAWS OF 1966 IN THE OPERATION OF THE ALCOHOL TEST 7110 MK III-C
A METHOD TO DETERMINE INTOXICATION
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, this 11th DAY OF March
TWO THOUSAND AND ELEVEN

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 1/17/13	OCPA	Adam Stankis
2. 1-22-15	OCPA	Wm. Ross
3. 4/26/17	LAKEHURST	Adam Stankis
4. 1-24-19	Lakehurst	R. J.
5. 8-5-21	Lakehurst	Dust
6. 3/24/23	Lakehurst	JAH
7.		
8.		
9.		
10.		

S.P. 293B (Rev. 03/10)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Pascal M. Gambardella, Jr.
Toms River Township
IS QUALIFIED AND COMPETENT TO CONDUCT CHIMIC BREATH ANALYSES PURSUANT TO CHAPTER 143 OF
THE LAWS OF 1966 IN THE OPERATION OF THE ALCOHOL TEST 7110 MK III-C
A METHOD TO DETERMINE INTOXICATION
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, this 13th DAY OF March
TWO THOUSAND AND THIRTEEN

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 3/3/15	OCPA	Adam Stankis
2. 4/27/17	LAKEHURST	Adam Stankis
3. 5/9/19	LAKEHURST	Adam Stankis
4. 7-9-21	Lakehurst	Hal Dulay
5. 3/3/23	Lakehurst	JAH
6.		
7.		
8.		
9.		
10.		

S.P. 293B (Rev. 03/10)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Michael P. Cassidy Jr.
Toms River Township
IS QUALIFIED AND COMPETENT TO CONDUCT CHIMIC BREATH ANALYSES PURSUANT TO CHAPTER 143 OF
THE LAWS OF 1966 IN THE OPERATION OF THE ALCOHOL TEST 7110 MK III-C
A METHOD TO DETERMINE INTOXICATION
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, this 23rd DAY OF May
TWO THOUSAND AND SIXTEEN

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES 08/26/2013 - 08/29/2013

DATE	Refresher Course PLACE	INSTRUCTOR
1. 02/03/2015	Ocean Co. P.A.	Stanks
2. 4-5-17	LAKEHURST	Wm. Ross
3. 4/16/19	LAKEHURST	Adam Stankis
4. 7-20-21	Lakehurst	Hal Dulay
5. 3/3/23	Lakehurst	JAH
6.		
7.		
8.		
9.		
10.		

S.P. 293B (Rev. 08/13)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Ryan P. Fitzgerald
Toms River Township

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1966 IN THE OPERATION OF THE **Alcotest 7110 MKIII-C**
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 25th DAY OF May

TWO THOUSAND AND Seventeen

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. <u>5/9/19</u>	<u>LAKEHURST</u>	<u>Odessa Stender</u>
2. <u>8-3-21</u>	<u>Lakehurst</u>	<u>Odessa Stender</u>
3. <u>2/28/23</u>	<u>Lakehurst</u>	<u>B. [Signature]</u>
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2938 (Rev. 08/16)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

John R. Marsicano
Toms River Township

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1966 IN THE OPERATION OF THE **Alcotest 7110 MKIII-C**
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 15th DAY OF February

TWO THOUSAND AND 18

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. <u>8/13/20</u>	<u>ALLU</u>	<u>Odessa Stender</u>
2. <u>4/21/22</u>	<u>Lakehurst</u>	<u>IFALL</u>
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2938 (Rev. 01/19)